

Sample Name: Indolicidin  
 Cat No. : RP11242  
 Lot No. : E1439420G  
 Time Processed: 1:30:24 AM  
 Month-Day-Year Processed :08/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

### <Chromatogram>

mV

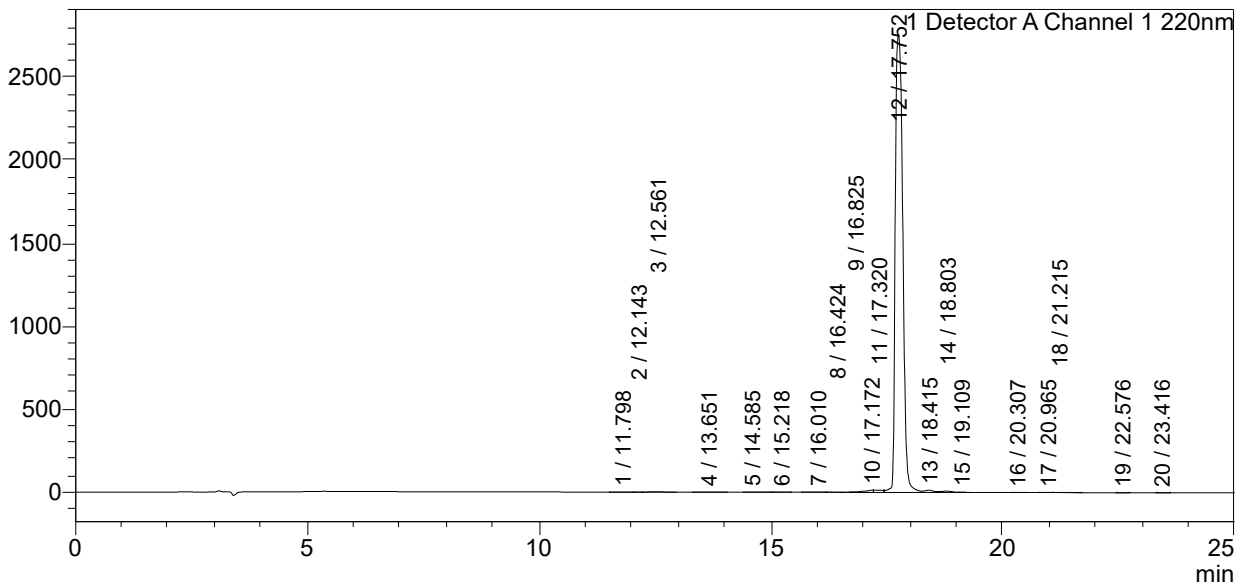

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.798	6136	323	0.019
2	12.143	5756	582	0.018
3	12.561	28296	1379	0.089
4	13.651	4108	199	0.013
5	14.585	5240	296	0.017
6	15.218	3968	445	0.013
7	16.010	10920	633	0.035
8	16.424	21028	1723	0.066
9	16.825	47007	3557	0.149
10	17.172	174548	12572	0.552
11	17.320	161844	13184	0.512
12	17.752	30815148	2759606	97.413
13	18.415	192850	12783	0.610
14	18.803	124443	8048	0.393

Peak#	Ret. Time	Area	Height	Area%
15	19.109	17254	1965	0.055
16	20.307	1083	144	0.003
17	20.965	3916	380	0.012
18	21.215	7492	556	0.024
19	22.576	1231	156	0.004
20	23.416	1128	143	0.004
Total		31633395	2818673	100.000