

Sample Name :LAH4
 Cat. No. : RP20096
 Lot. No. : E7493619F
 Time Processed : 8:59:39
 Month-Day-Year Processed : 06/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

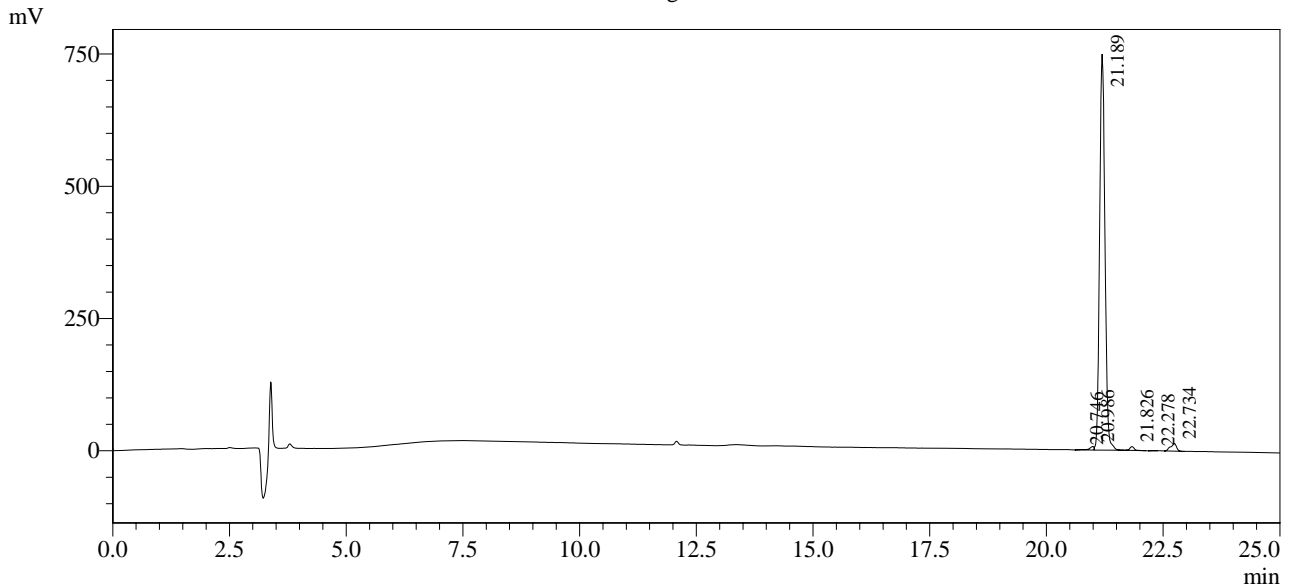

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	20.746	7038	865	0.114
2	20.986	41622	6504	0.672
3	21.189	5973137	748232	96.384
4	21.826	45383	7328	0.732
5	22.278	1089	221	0.018
6	22.734	128962	14625	2.081
Total		6197231	777774	100.000