

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), human
 Cat No. : RP11089
 Lot No. : E0541420J
 Time Processed : 9:14:59
 Month-Day-Year Processed : 10/27/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

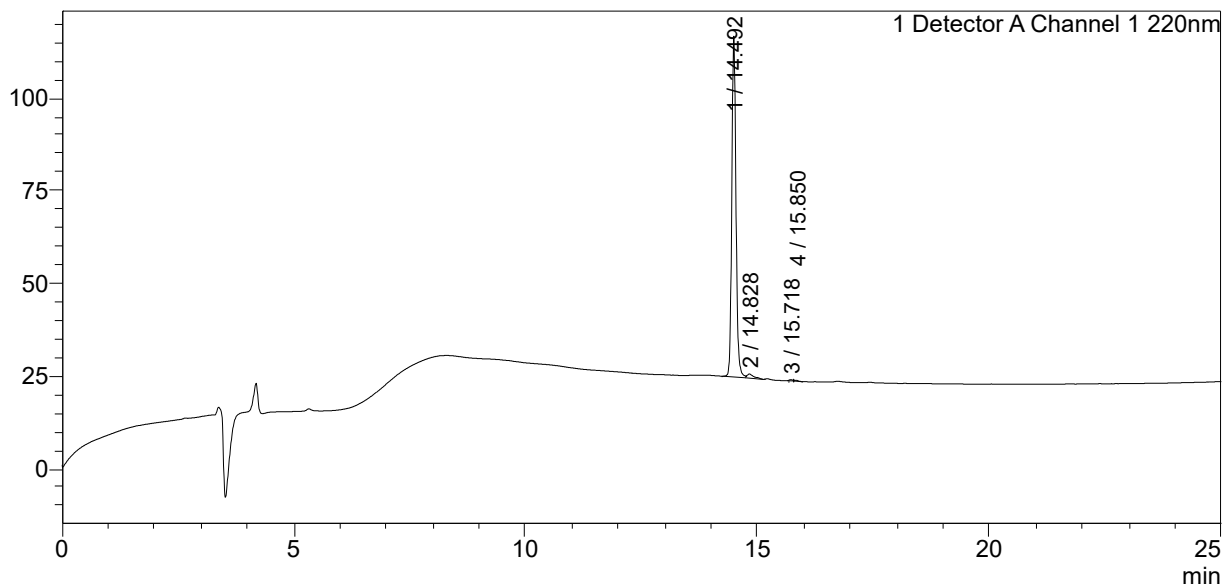

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.492	575748	92004	97.507
2	14.828	11819	1133	2.002
3	15.718	1783	326	0.302
4	15.850	1116	218	0.189
Total		590465	93681	100.000