

Sample Name :HIF-1 alpha (556-574)  
 Cat No.: RP20479  
 Lot No.:E9040719I  
 Time Processed :13:25:15  
 Month-Day-Year Processed :09/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

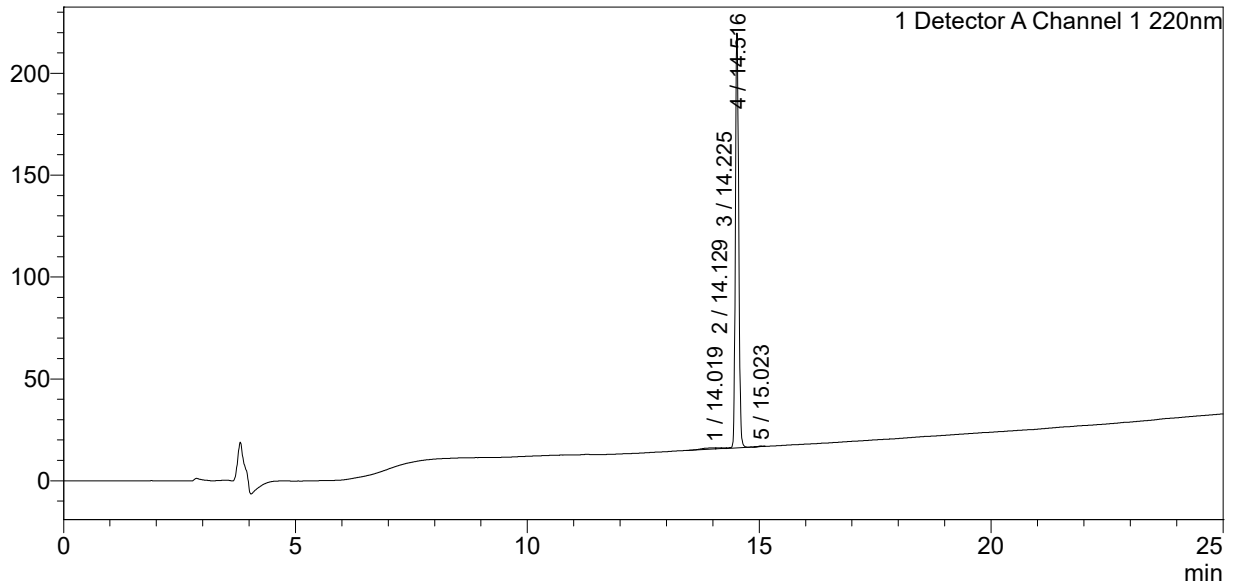

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.019	14170	608	1.376
2	14.129	3333	483	0.324
3	14.225	2195	353	0.213
4	14.516	1007938	203692	97.914
5	15.023	1778	324	0.173
Total		1029414	205461	100.000