

Sample Name : C-Type Natriuretic Peptide (CNP) (1-22), human  
 Cat No.: RP11110  
 Lot No.: E38669201  
 Time Processed :9:57:13  
 Month-Day-Year Processed :08/25/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

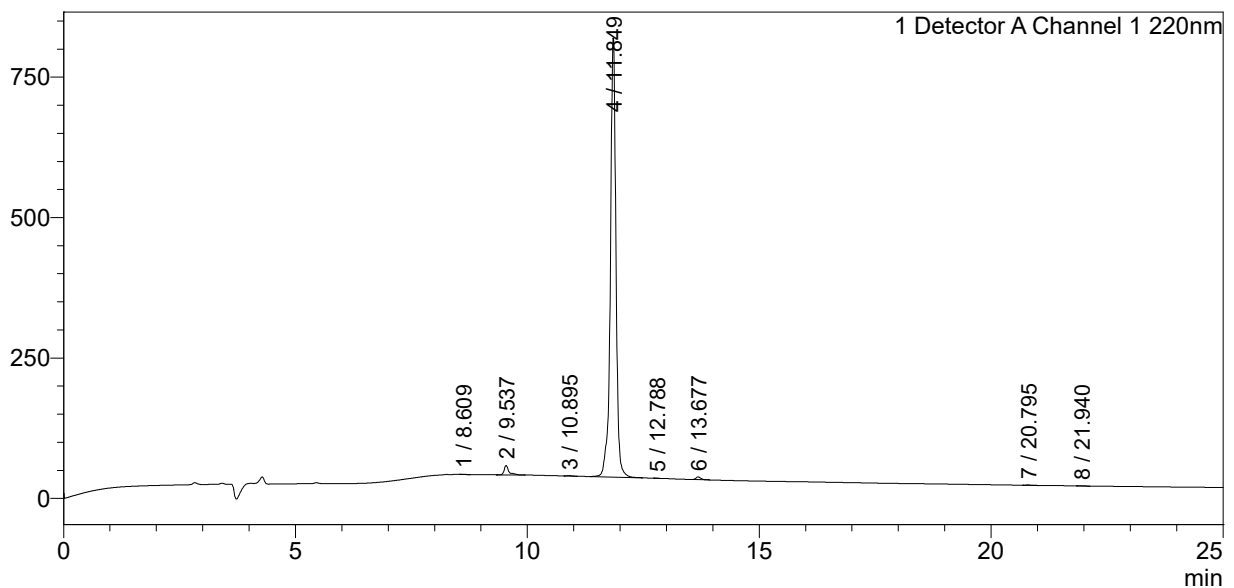

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.609	2337	464	0.035
2	9.537	121929	16907	1.819
3	10.895	4852	662	0.072
4	11.849	6528492	781846	97.418
5	12.788	2010	411	0.030
6	13.677	35249	4913	0.526
7	20.795	4271	549	0.064
8	21.940	2387	384	0.036
Total		6701527	806138	100.000