

Sample Name : $\beta$ -Amyloid (1-42), human  
 Cat No. :RP20527  
 Lot No. :E0204320B  
 Time Processed :14:27:47  
 Month-Day-Year Processed :03/25/2020

Pump A : 0.5% Ammonia solution in 100% water (v/v)  
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

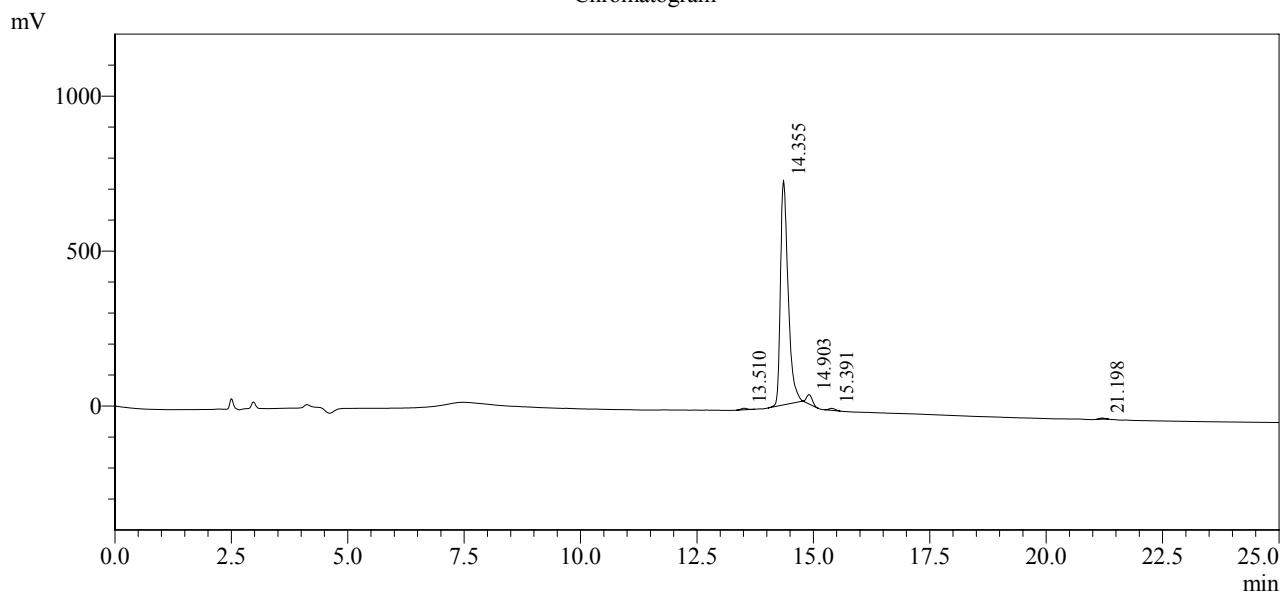

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.510	46888	4999	0.538
2	14.355	8316506	725881	95.508
3	14.903	257236	30219	2.954
4	15.391	58633	6213	0.673
5	21.198	28372	3475	0.326
Total		8707635	770787	100.000