

Sample Name: GRGDSP

Cat. No. : RP20255

Lot. No. : E7260919I

Time Processed: 8:23:37 AM

Month-Day-Year

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 5 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Controller | Stop | |

<<Column Performance>>


<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Equipment:ZJ19010325

<Chromatogram>

mV

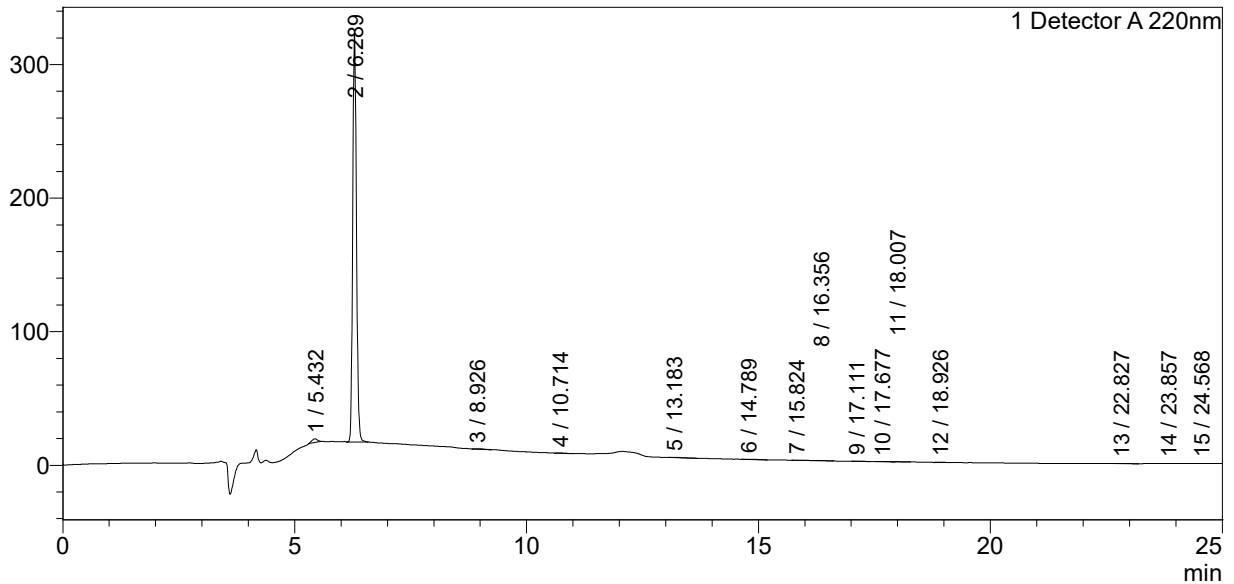

<Peak Table>

Detector A 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 5.432 | 23965 | 2825 | 1.350 |
| 2 | 6.289 | 1724564 | 306136 | 97.171 |
| 3 | 8.926 | 5250 | 380 | 0.296 |
| 4 | 10.714 | 2227 | 196 | 0.125 |
| 5 | 13.183 | 3552 | 184 | 0.200 |
| 6 | 14.789 | 3011 | 164 | 0.170 |
| 7 | 15.824 | 2275 | 84 | 0.128 |
| 8 | 16.356 | 1119 | 88 | 0.063 |
| 9 | 17.111 | 1608 | 123 | 0.091 |
| 10 | 17.677 | 1259 | 105 | 0.071 |
| 11 | 18.007 | 1135 | 102 | 0.064 |
| 12 | 18.926 | 1033 | 107 | 0.058 |
| 13 | 22.827 | 1153 | 59 | 0.065 |
| 14 | 23.857 | 1290 | 75 | 0.073 |
| 15 | 24.568 | 1324 | 81 | 0.075 |
| Total | | 1774766 | 310708 | 100.000 |