


Mass Spectrum

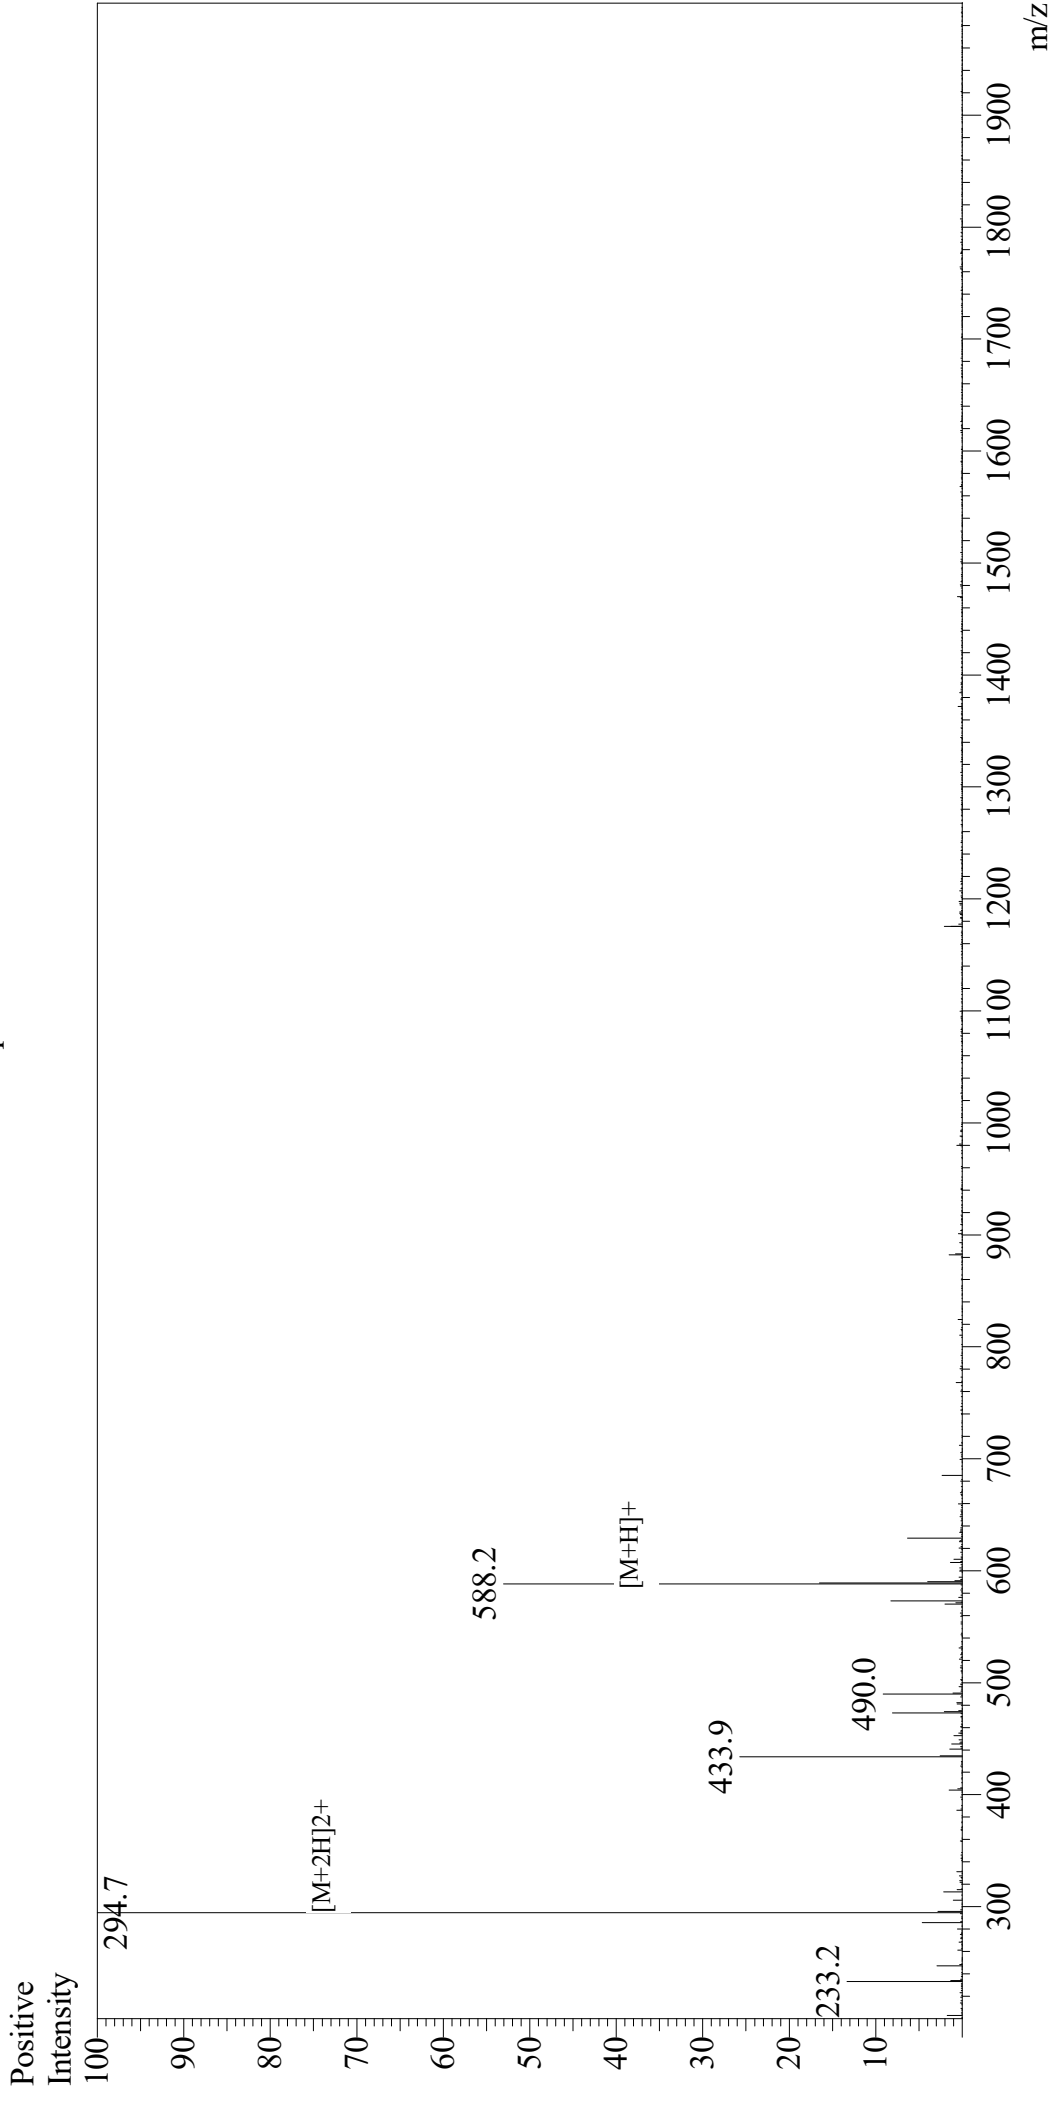

Sample Information

User : Gary  
Month-Day Processed : 09/05/19  
Time Processed : 08:38:24 AM  
Injection Volume : 0.3  
Sample Name : GRGDSP  
Cat No. : RP20255  
Lot No. : E7260919I  
Theoretical MW : 587.59  
Observed MW : 587.4

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200  
Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H<sub>2</sub>O/50%MeOH