

Sample Name : Calcitonin, eel
 Cat No.: RP12786
 Lot No.: E2784720D
 Time Processed : 4:29:35
 Month-Day-Year Processed : 04/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

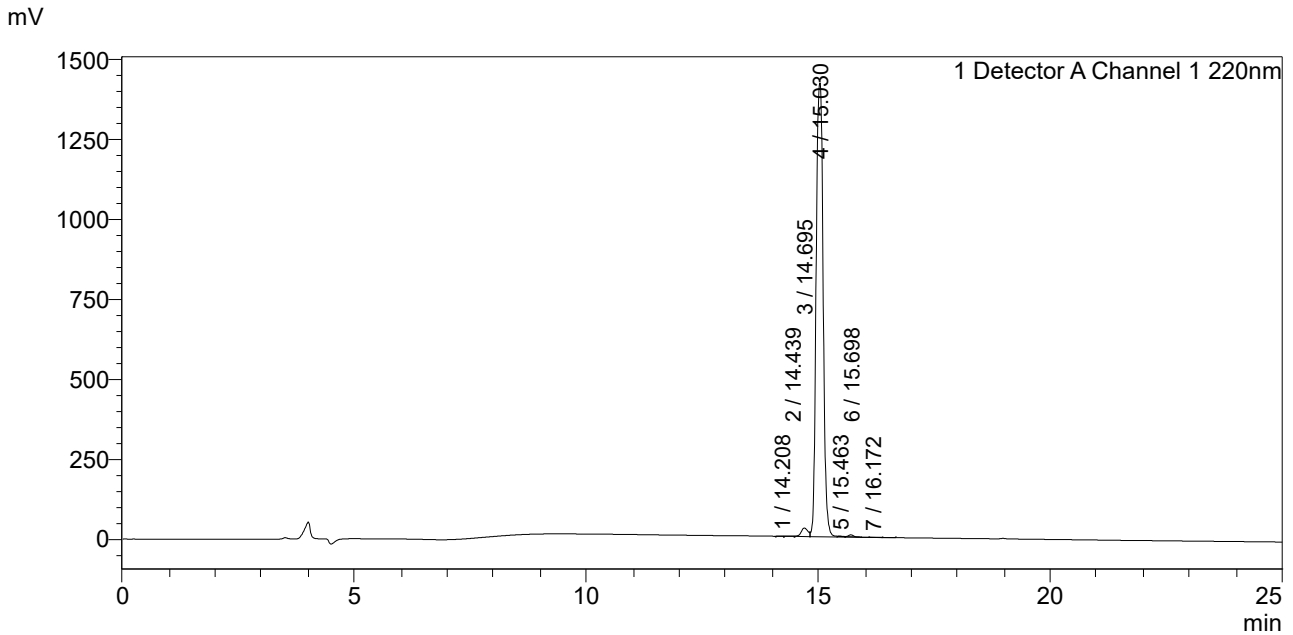

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.208	2940	424	0.019
2	14.439	19127	1634	0.126
3	14.695	273375	26902	1.804
4	15.030	14809100	1422980	97.727
5	15.463	2529	441	0.017
6	15.698	42461	6096	0.280
7	16.172	4057	453	0.027
Total		15153588	1458929	100.000