

Sample Name : β -Amyloid (15-21)
 Cat. No. : RP20171
 Lot. No. : E6794219J
 Time Processed :21:07:27
 Month-Day-Year Processed :10/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

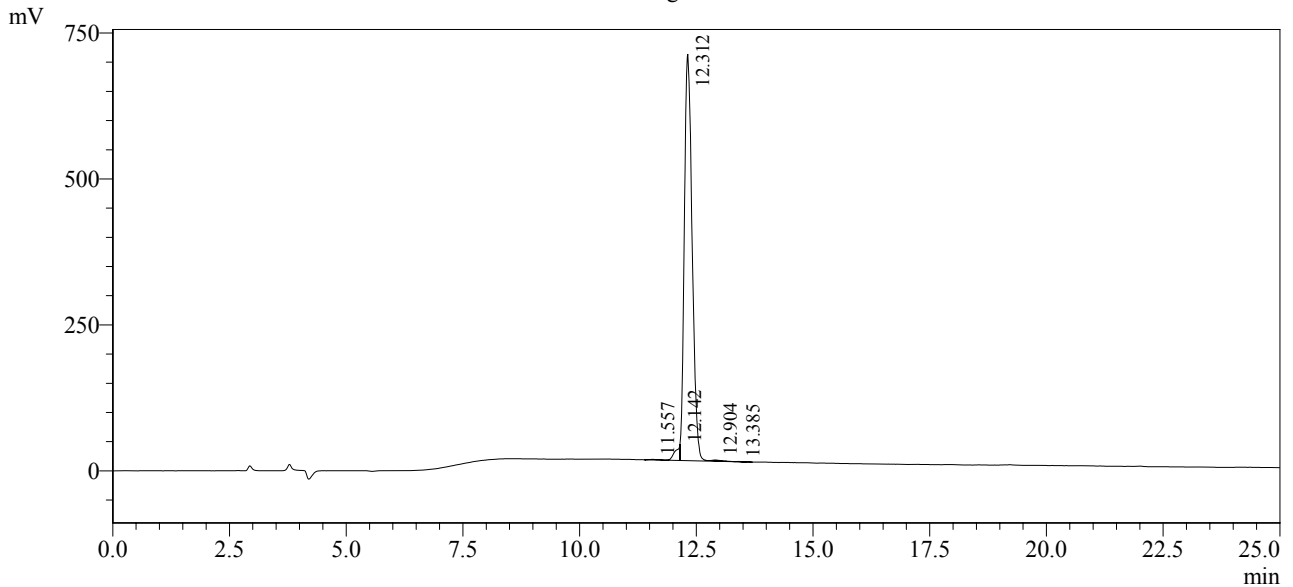

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.557	14676	1038	0.176
2	12.142	187256	23862	2.242
3	12.312	8137109	696233	97.433
4	12.904	11073	1328	0.133
5	13.385	1378	436	0.017
Total		8351491	722897	100.000