

Sample Name :  $\beta$ -Amyloid (25-35)  
 Cat. No. : RP10008  
 Lot. No. : E6983520D  
 Time Processed :8:45:41  
 Month-Day-Year Processed :04/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GR11010440

Chromatogram

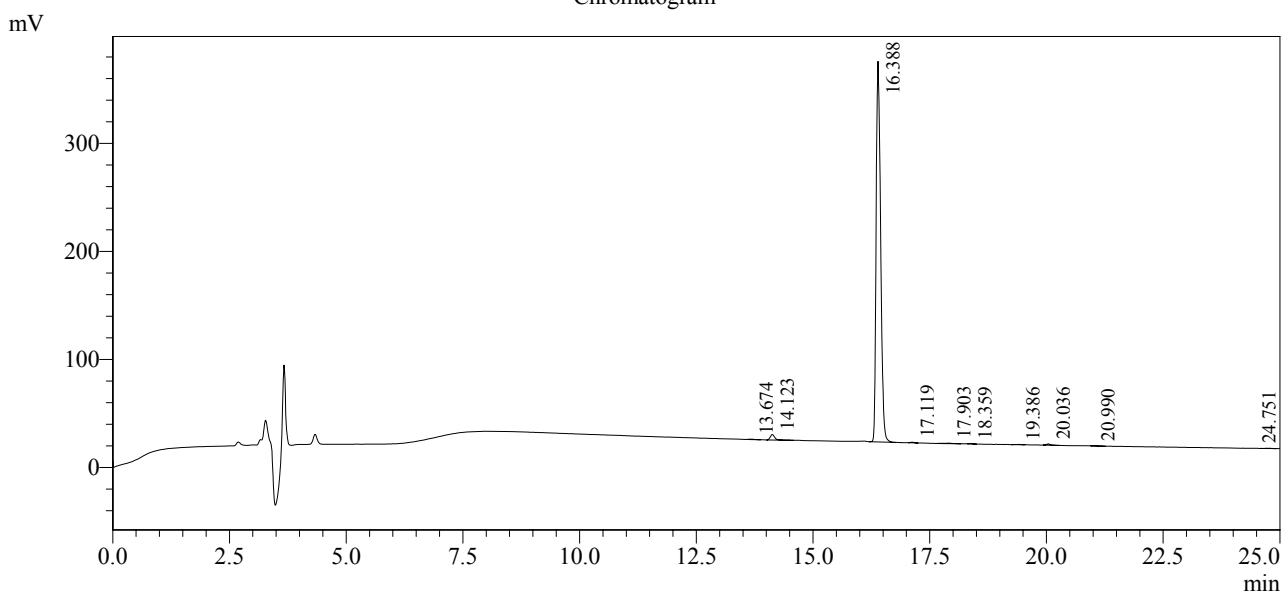

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.674	2512	395	0.103
2	14.123	34144	5060	1.407
3	16.388	2368275	352375	97.571
4	17.119	3071	631	0.127
5	17.903	5120	415	0.211
6	18.359	1075	216	0.044
7	19.386	1895	244	0.078
8	20.036	7274	1236	0.300
9	20.990	1192	133	0.049
10	24.751	2673	295	0.110
Total		2427231	361000	100.000