


Mass Spectrum

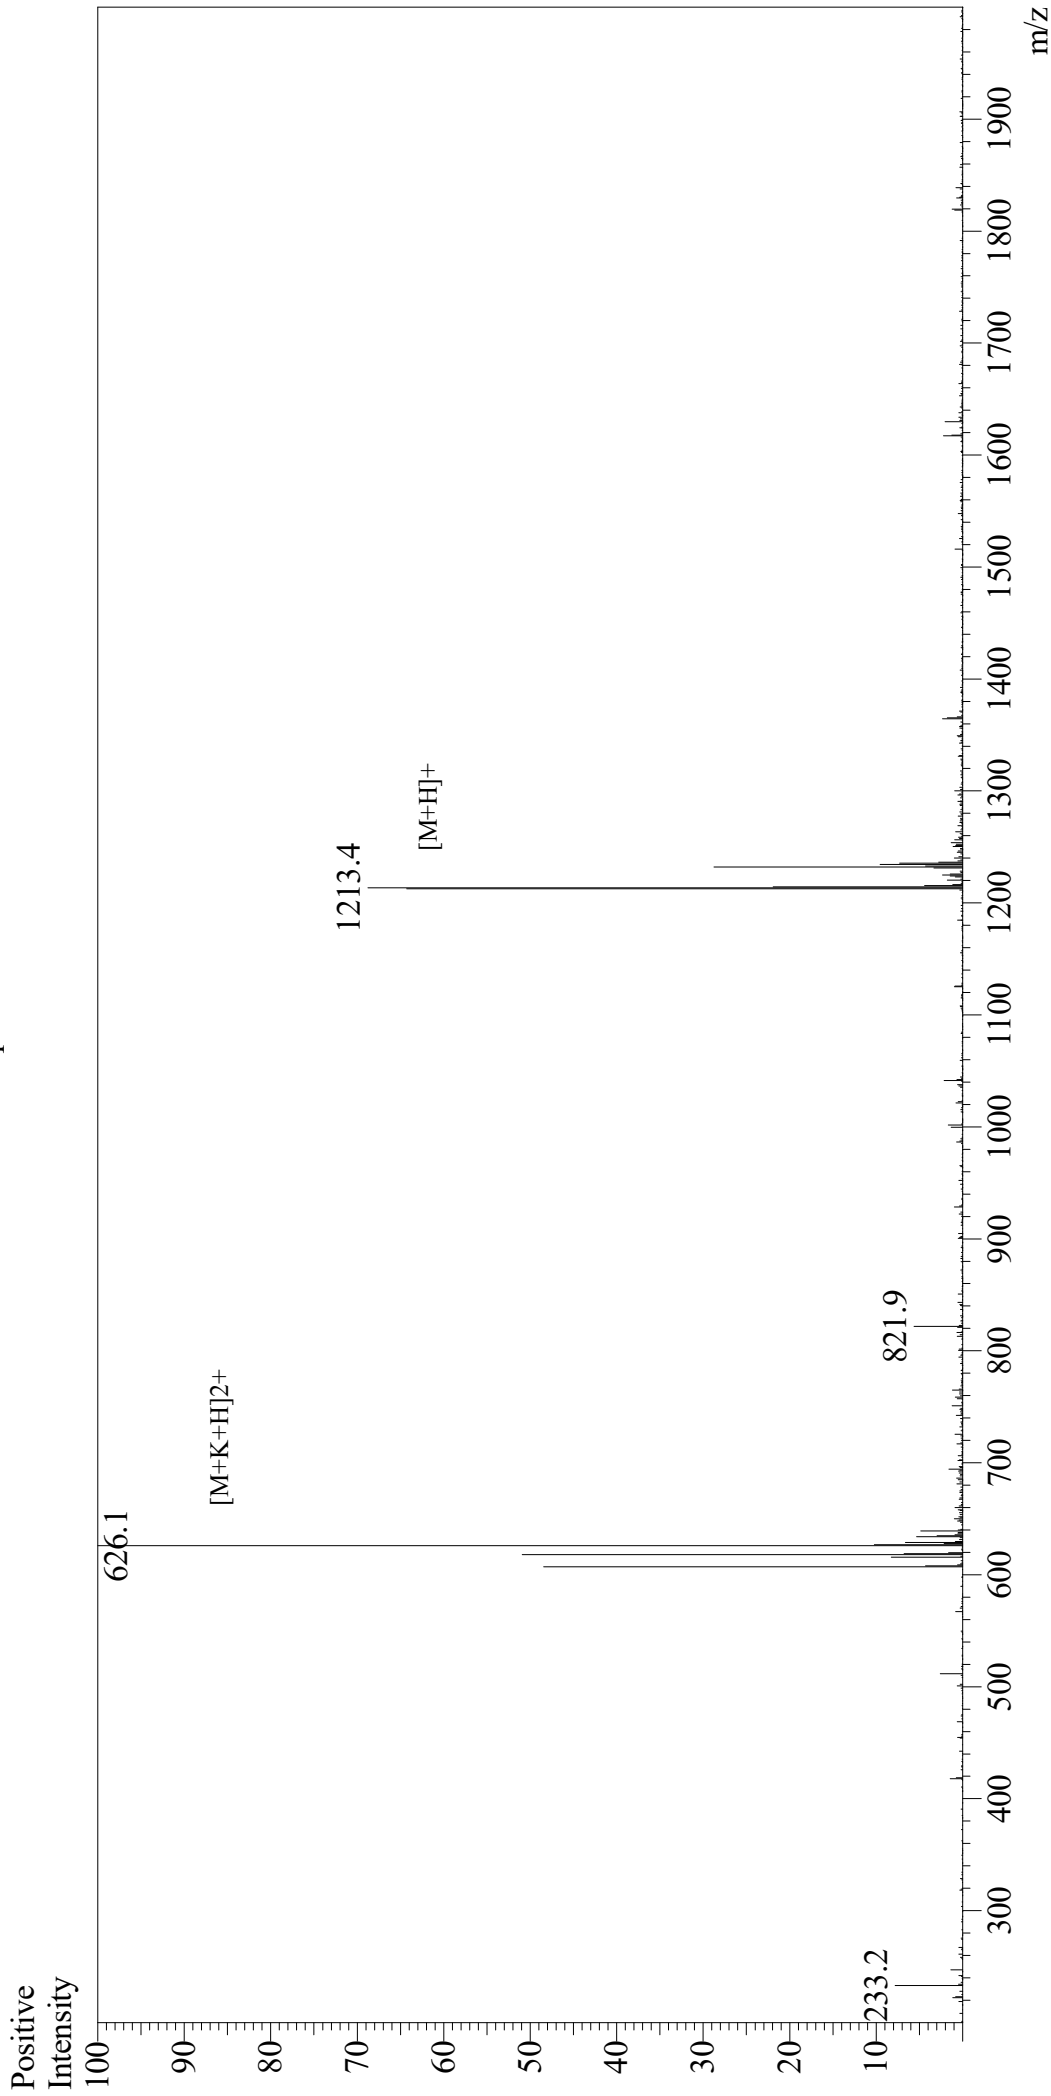

Sample Information

User : Gary
Month-Day Processed : 02/16/19
Time Processed : 07:13:00 PM
Injection Volume : 0.2
Sample Name : Luteinizing Hormone Releasing Hormone (LH-RH), salmon
Cat No. : RP10673
Lot No. : PE3261901
Theoretical MW : 1212.31
Observed MW : 1213.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH