

Sample Name : Endothelin 1, human, porcine
 Cat No. : RP12758
 Lot No. : E8068621C
 Time Processed : 4:30:28 AM
 Month-Day-Year Processed : 03/11/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : ZJ19010140

<Chromatogram>

mV

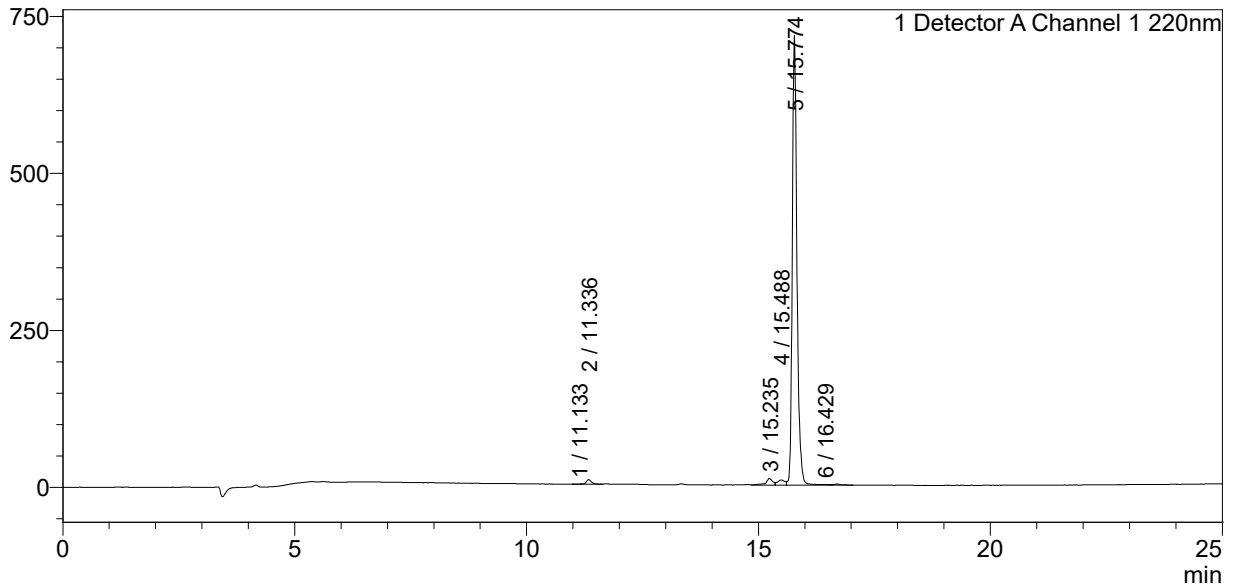

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.133	2076	269	0.039
2	11.336	61697	7387	1.160
3	15.235	109906	10730	2.066
4	15.488	89219	8123	1.677
5	15.774	5056053	715911	95.032
6	16.429	1398	177	0.026
Total		5320349	742597	100.000