

Sample Name :HIV p17 Gag (77-85)
 Cat. No. : RP17316
 Lot. No. : E4898319I
 Time Processed :20:22:17
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01 | Pumps | Pump B Conc. | 5 | |
| 25.00 | Pumps | Pump B Conc. | 65 | |
| 25.01 | Pumps | Pump B Conc. | 95 | |
| 27.00 | Pumps | Pump B Conc. | 95 | |
| 27.01 | Pumps | Pump B Conc. | 5 | |
| 35.00 | Pumps | Pump B Conc. | 5 | |
| 35.01 | Controller | Stop | | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

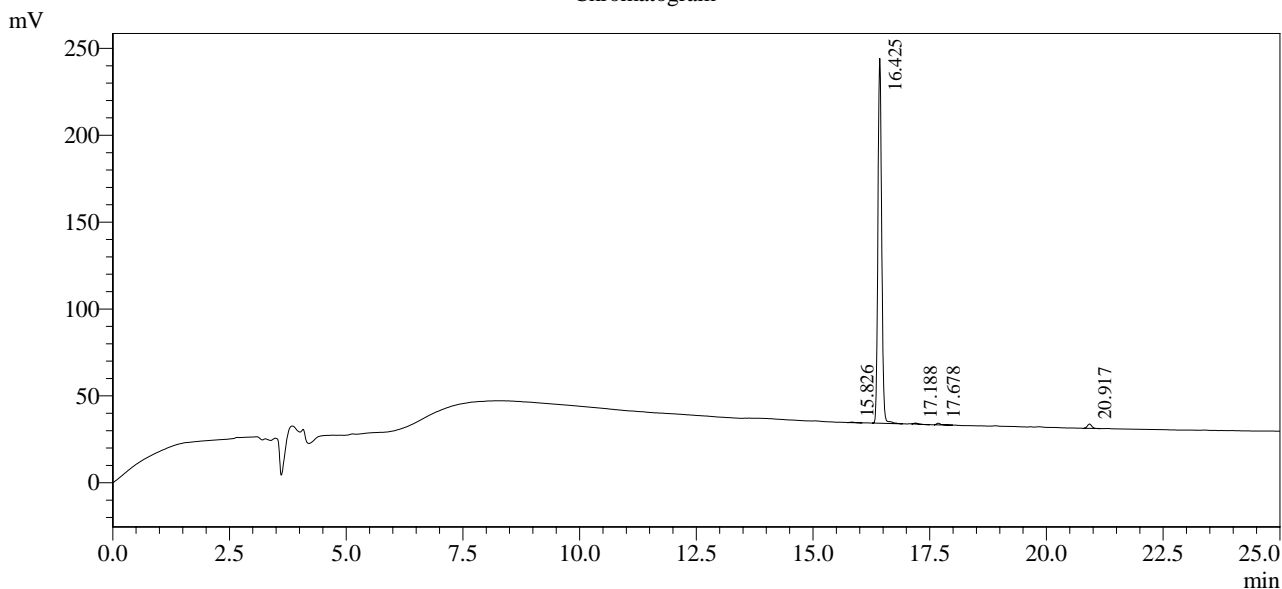

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 15.826 | 1991 | 287 | 0.165 |
| 2 | 16.425 | 1182130 | 210080 | 97.713 |
| 3 | 17.188 | 3803 | 587 | 0.314 |
| 4 | 17.678 | 5950 | 930 | 0.492 |
| 5 | 20.917 | 15924 | 2483 | 1.316 |
| Total | | 1209798 | 214367 | 100.000 |