


Mass Spectrum

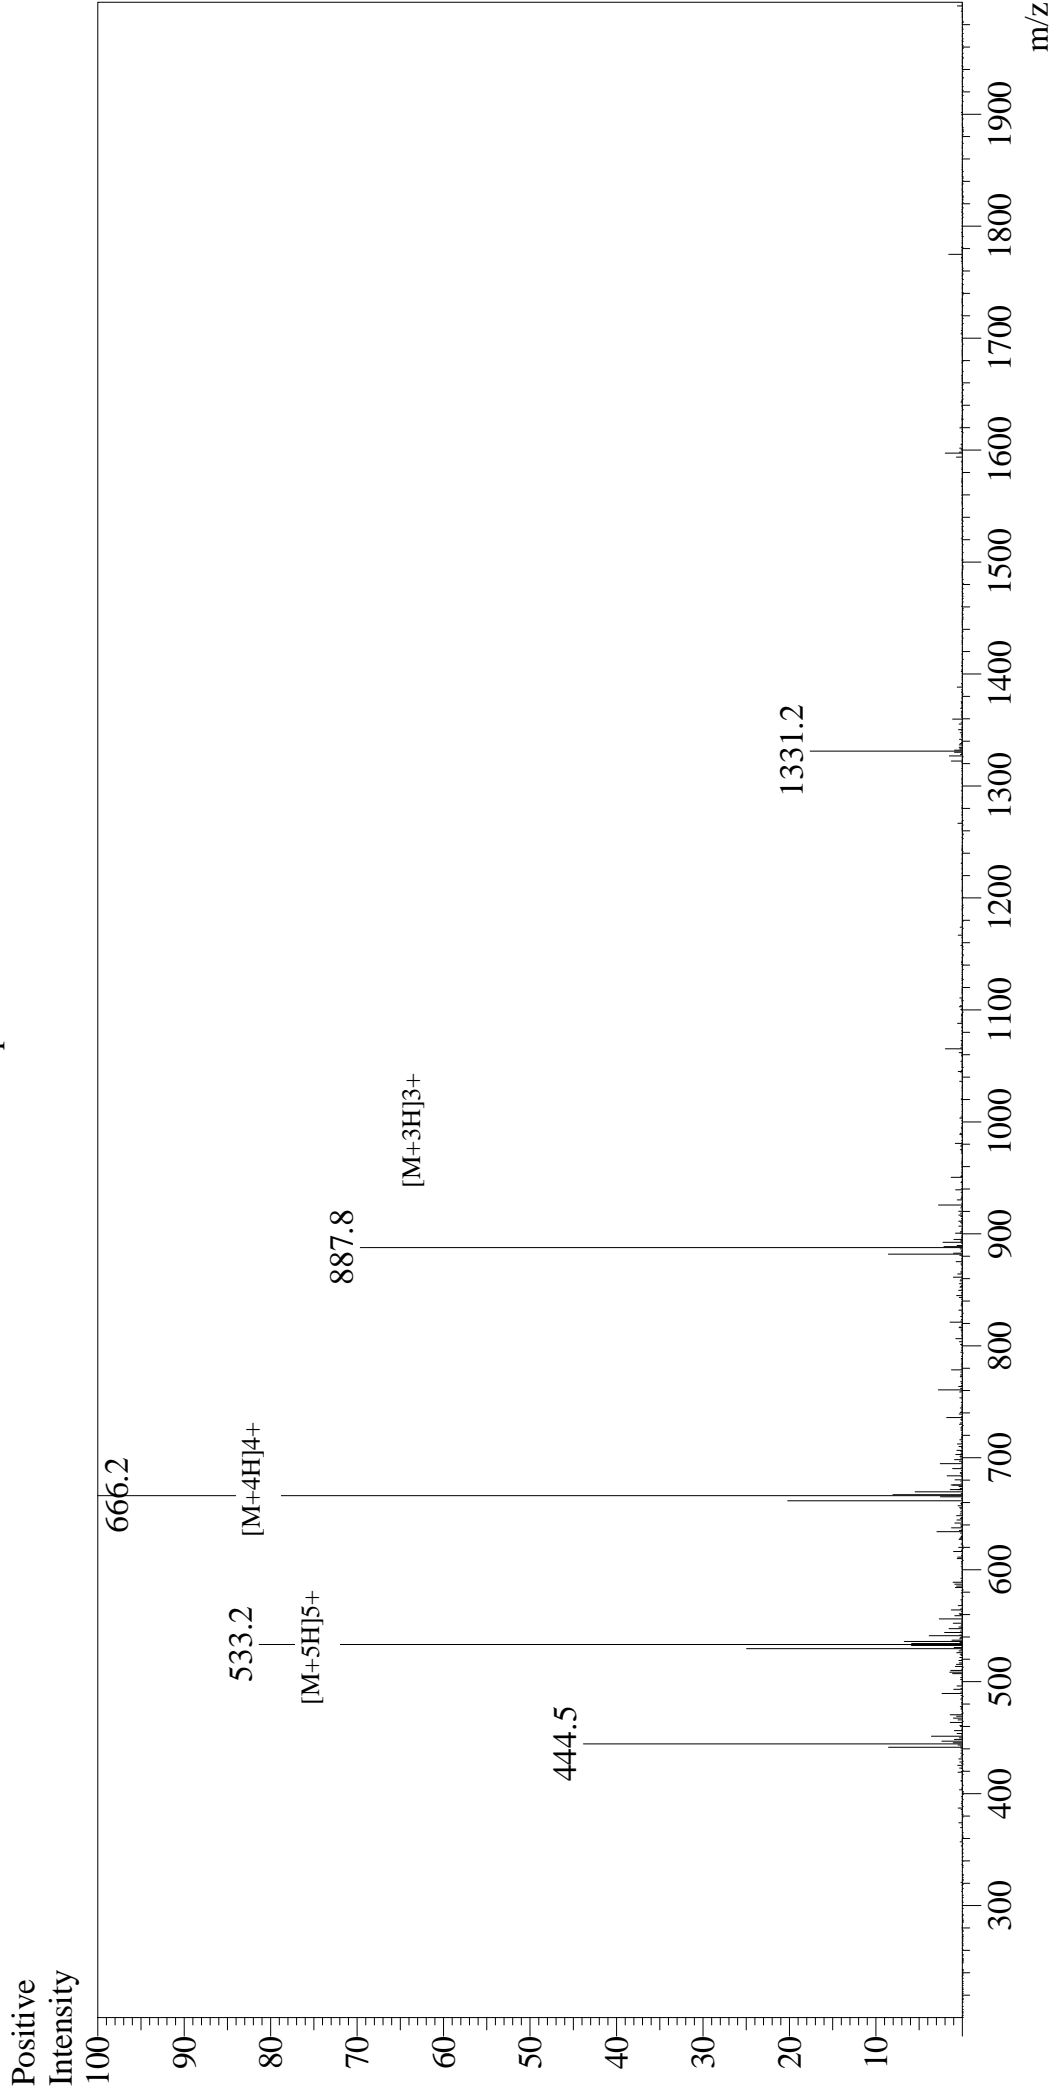

Sample Information

User : Gary
Month-Day Processed : 11/13/19
Time Processed : 21:03:27
Injection Volume : 0.3
Sample Name : ?-Melanocyte Stimulating Hormone (MSH), human
Cat No. : RP10648
Lot No. : E4566419K
Theoretical MW : 2661.00
Observed MW : 2660.8

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH