

Sample Name : p2Ca
 Cat. No. : RP19988
 Lot. No. : PE8631902
 Time Processed : 14:43:19
 Month-Day-Year Processed : 03/08/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

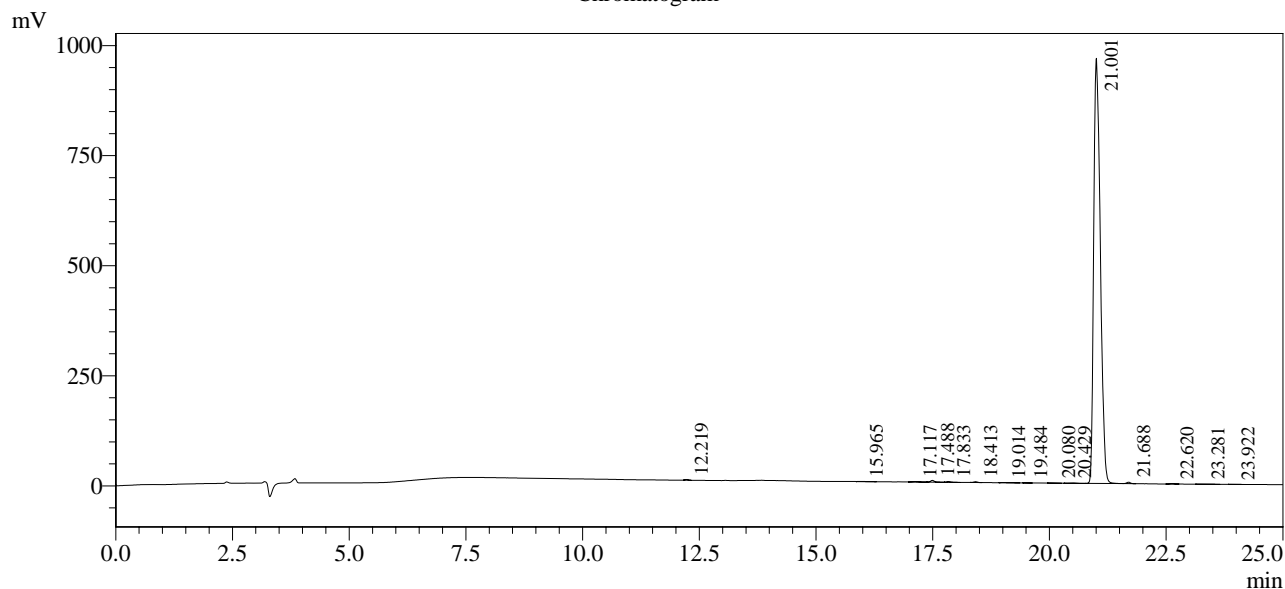

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.219	6930	1544	0.072
2	15.965	3710	404	0.039
3	17.117	6932	797	0.072
4	17.488	23715	4066	0.247
5	17.833	9149	1468	0.095
6	18.413	9875	1779	0.103
7	19.014	4445	516	0.046
8	19.484	1360	251	0.014
9	20.080	2327	245	0.024
10	20.429	7335	620	0.076
11	21.001	9503998	965814	98.896
12	21.688	19140	3302	0.199
13	22.620	5757	938	0.060
14	23.281	3645	213	0.038
15	23.922	1785	167	0.019
Total		9610104	982124	100.000