

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E6899719K
 Time Processed :10:18:03 AM
 Month-Day-Year Processed :11/09/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

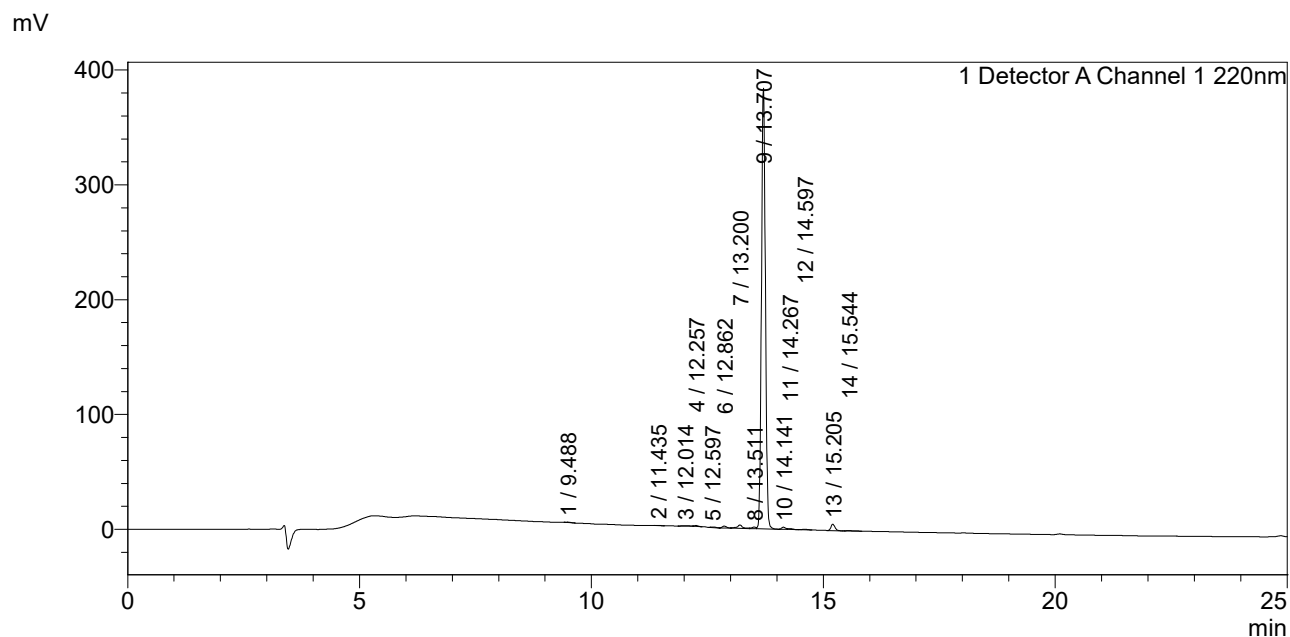

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.488	2769	433	0.116
2	11.435	1055	173	0.044
3	12.014	3476	370	0.146
4	12.257	3294	678	0.138
5	12.597	3747	475	0.157
6	12.862	10068	1670	0.422
7	13.200	23639	2902	0.990
8	13.511	8054	1368	0.337
9	13.707	2277469	383916	95.348
10	14.141	11161	1859	0.467
11	14.267	5612	821	0.235
12	14.597	3396	480	0.142
13	15.205	32628	5532	1.366
14	15.544	2213	226	0.093
Total		2388582	400903	100.000