

Sample Name : SAMs Peptide
 Cat No : RP10172
 Lot No : E2655721E
 Time Processed : 20:26:53
 Month-Day-Year Processed : 05/07/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : SS-CM-0309

<Chromatogram>

mV

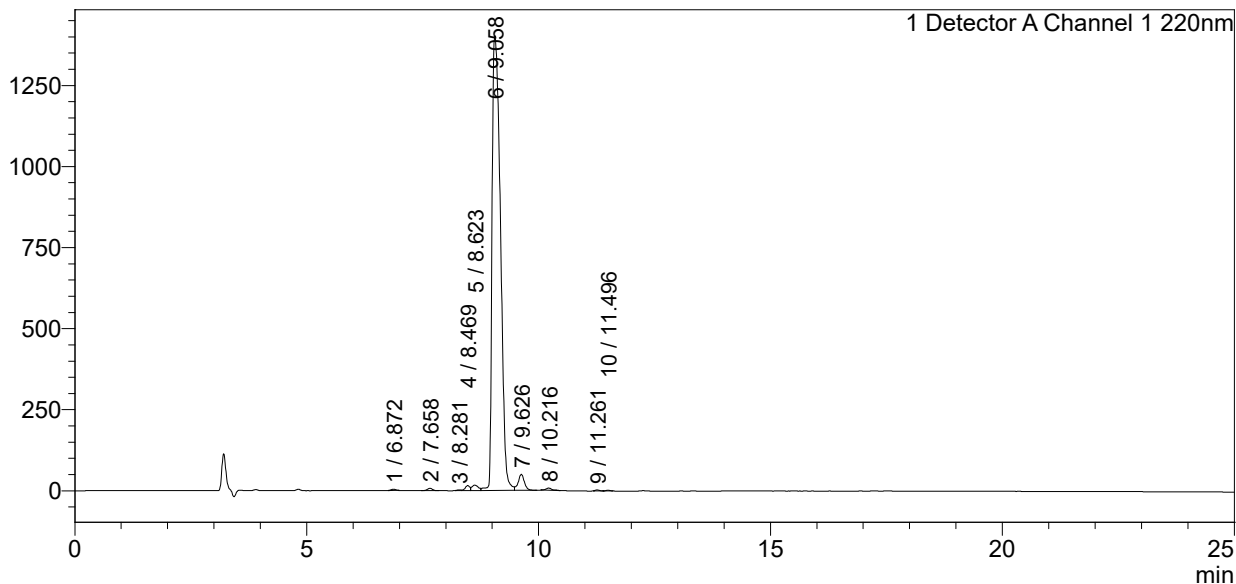

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.872	24921	3692	0.135
2	7.658	57345	7361	0.312
3	8.281	12271	2087	0.067
4	8.469	102504	15266	0.557
5	8.623	158999	16392	0.864
6	9.058	17497407	1402888	95.104
7	9.626	454694	49452	2.471
8	10.216	60667	6661	0.330
9	11.261	16659	2794	0.091
10	11.496	12796	2191	0.070
Total		18398263	1508785	100.000