

Sample Information

Sample Name :Rhodopsin Epitope Tag  
 Cat. No. : RP20400  
 Lot. No. : PE6531809

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>  
 Flow : 1.0000 mL/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>  
 <Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm

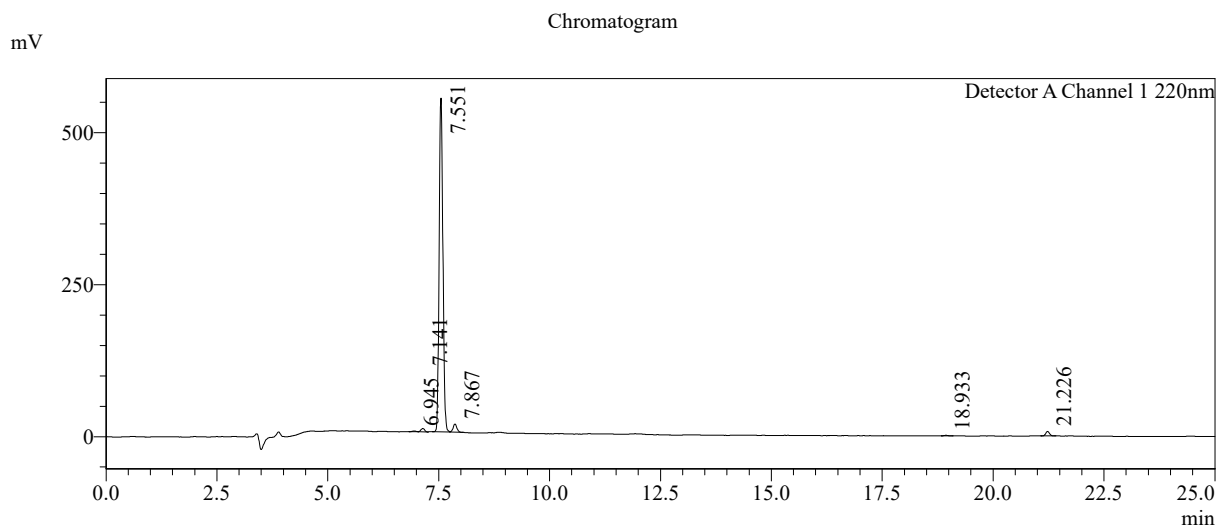

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	6.945	1297	7604	0.224	0.223
2	7.141	5706	32056	0.988	0.940
3	7.551	549044	3242299	95.037	95.032
4	7.867	13425	80208	2.324	2.351
5	18.933	930	5780	0.161	0.169
6	21.226	7316	43845	1.266	1.285
Total		577718	3411793	100.000	100.000