


Mass Spectrum

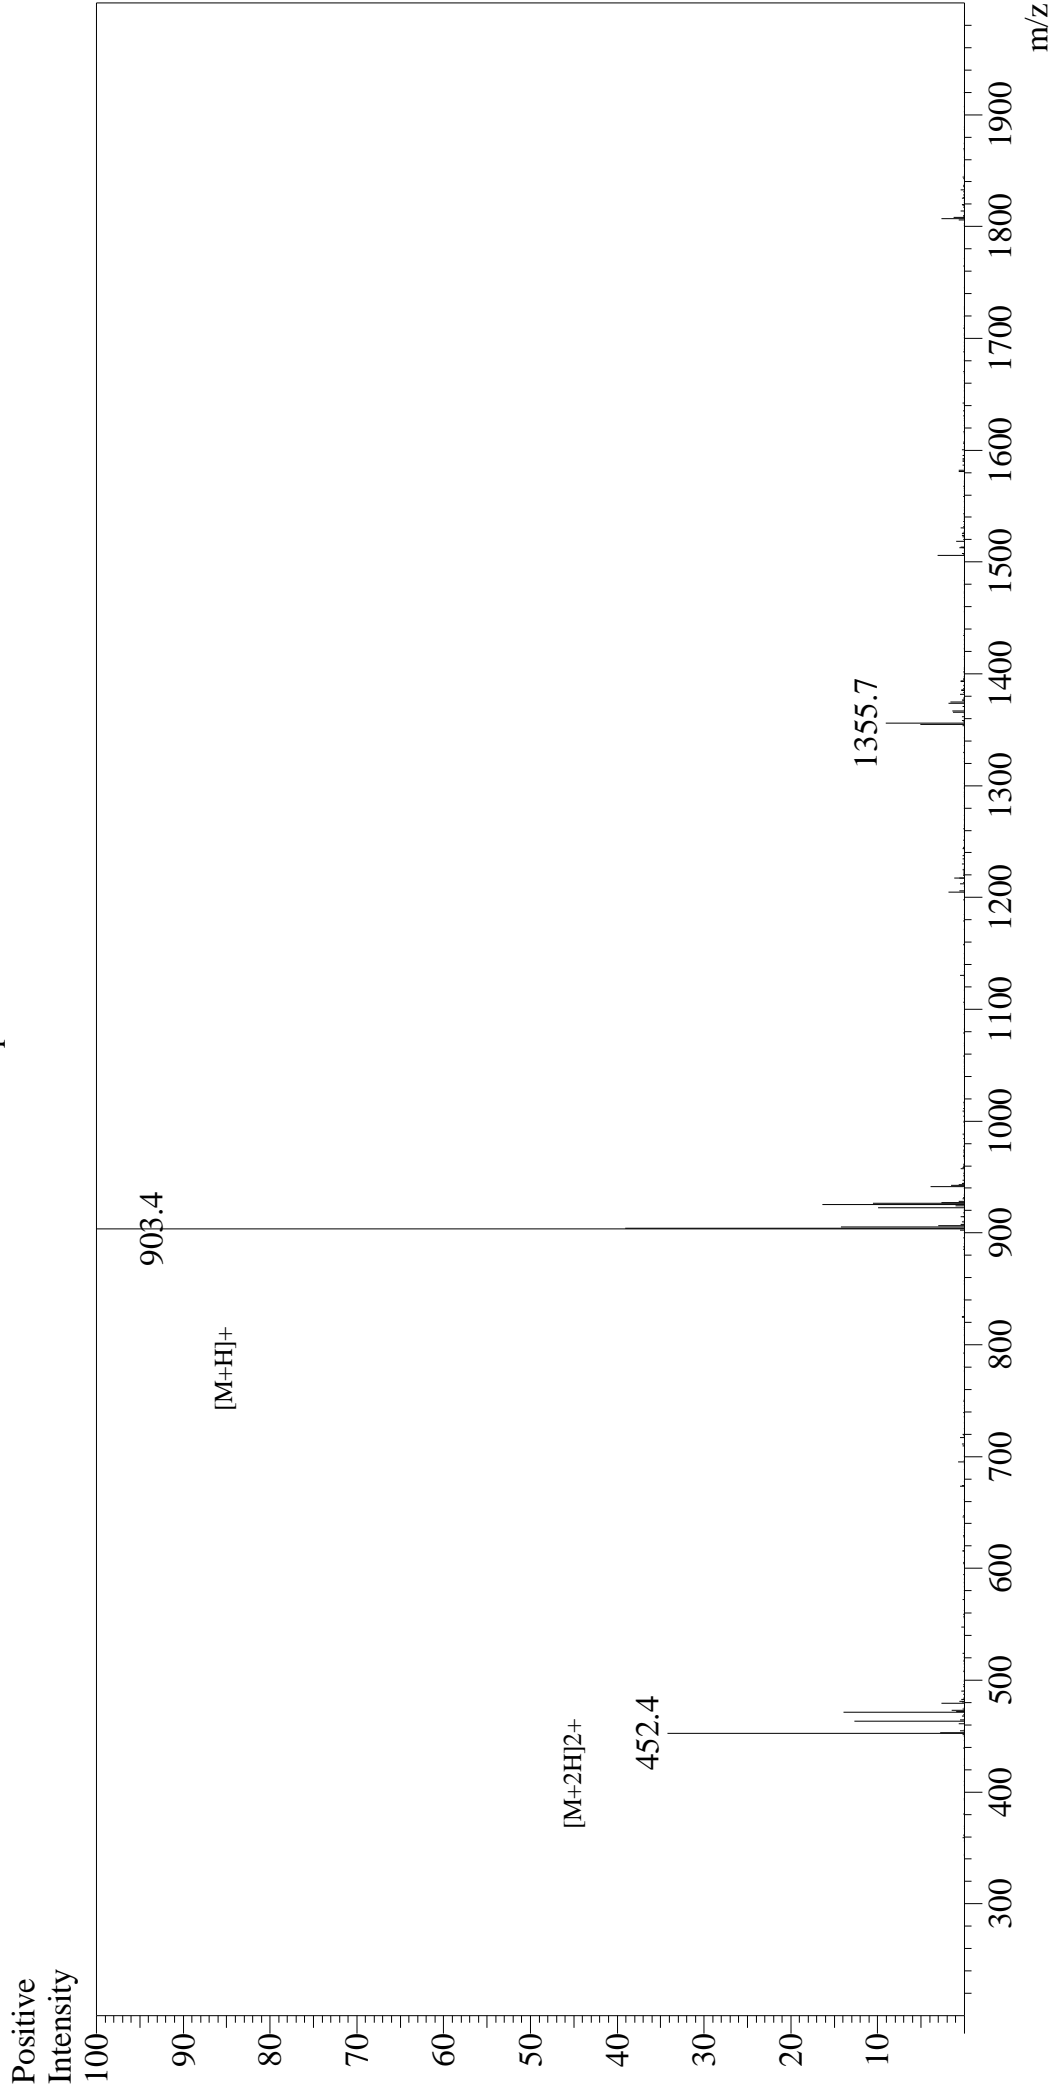

Sample Information

User : Gary
Month-Day Processed : 09/14/18
Time Processed : 13:34:07
Injection Volume : 0.2
Sample Name : Rhodopsin Epitope Tag
Cat No. : RP20400
Lot No. : PE6531809
Theoretical MW : 902.95
Observed MW : 902.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH