

Sample Name :AMARA peptide  
 Cat No. :RP20472  
 Lot No. :E4982719I  
 Time Processed :9:46:38 AM  
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

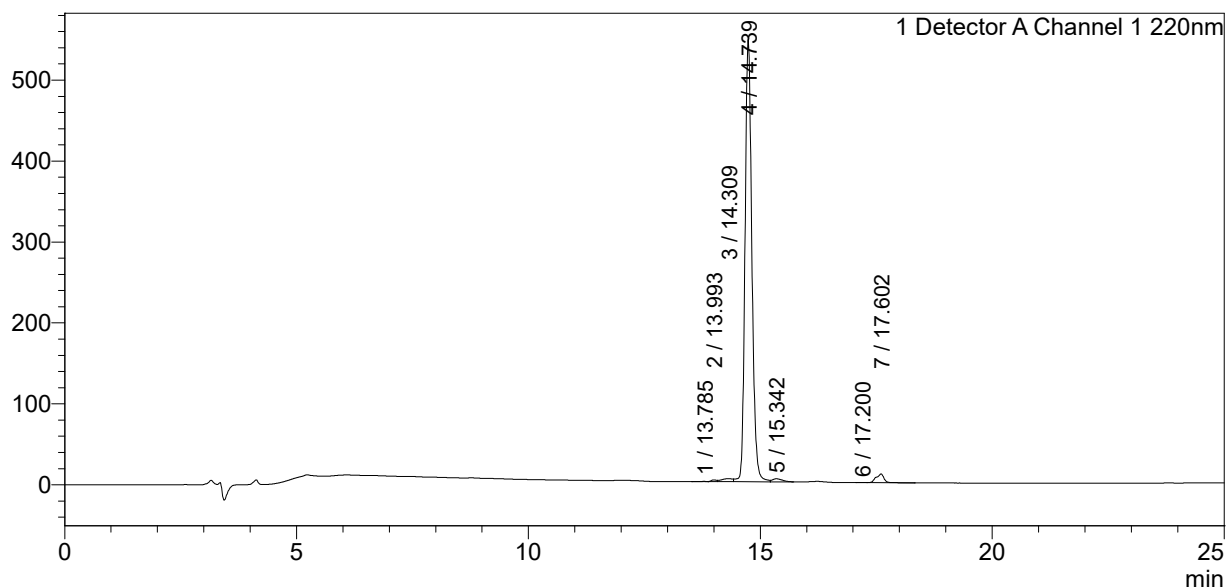

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.785	3344	344	0.057
2	13.993	18233	2288	0.311
3	14.309	63064	3732	1.074
4	14.739	5603173	546977	95.421
5	15.342	53210	3764	0.906
6	17.200	1527	163	0.026
7	17.602	129522	10869	2.206
Total		5872071	568138	100.000