

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :PE6141901
 Time Processed :3:32:37
 Month-Day-Year Processed :01/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

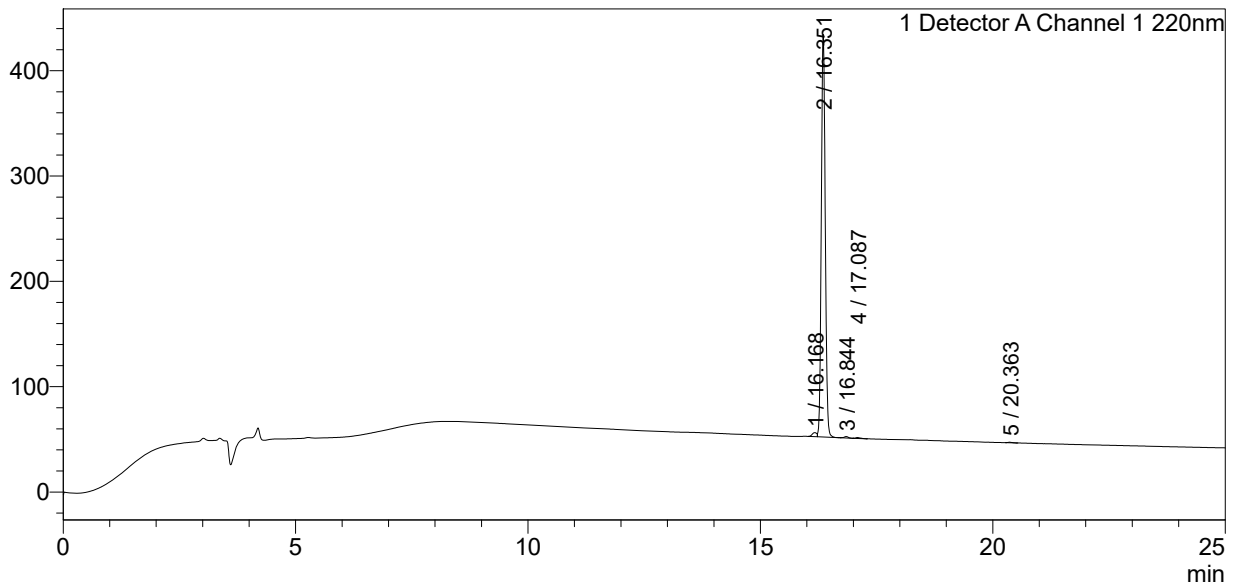

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.168	26500	3874	1.154
2	16.351	2253259	382152	98.107
3	16.844	8117	1356	0.353
4	17.087	5835	831	0.254
5	20.363	3027	490	0.132
Total		2296738	388702	100.000