


# Mass Spectrum

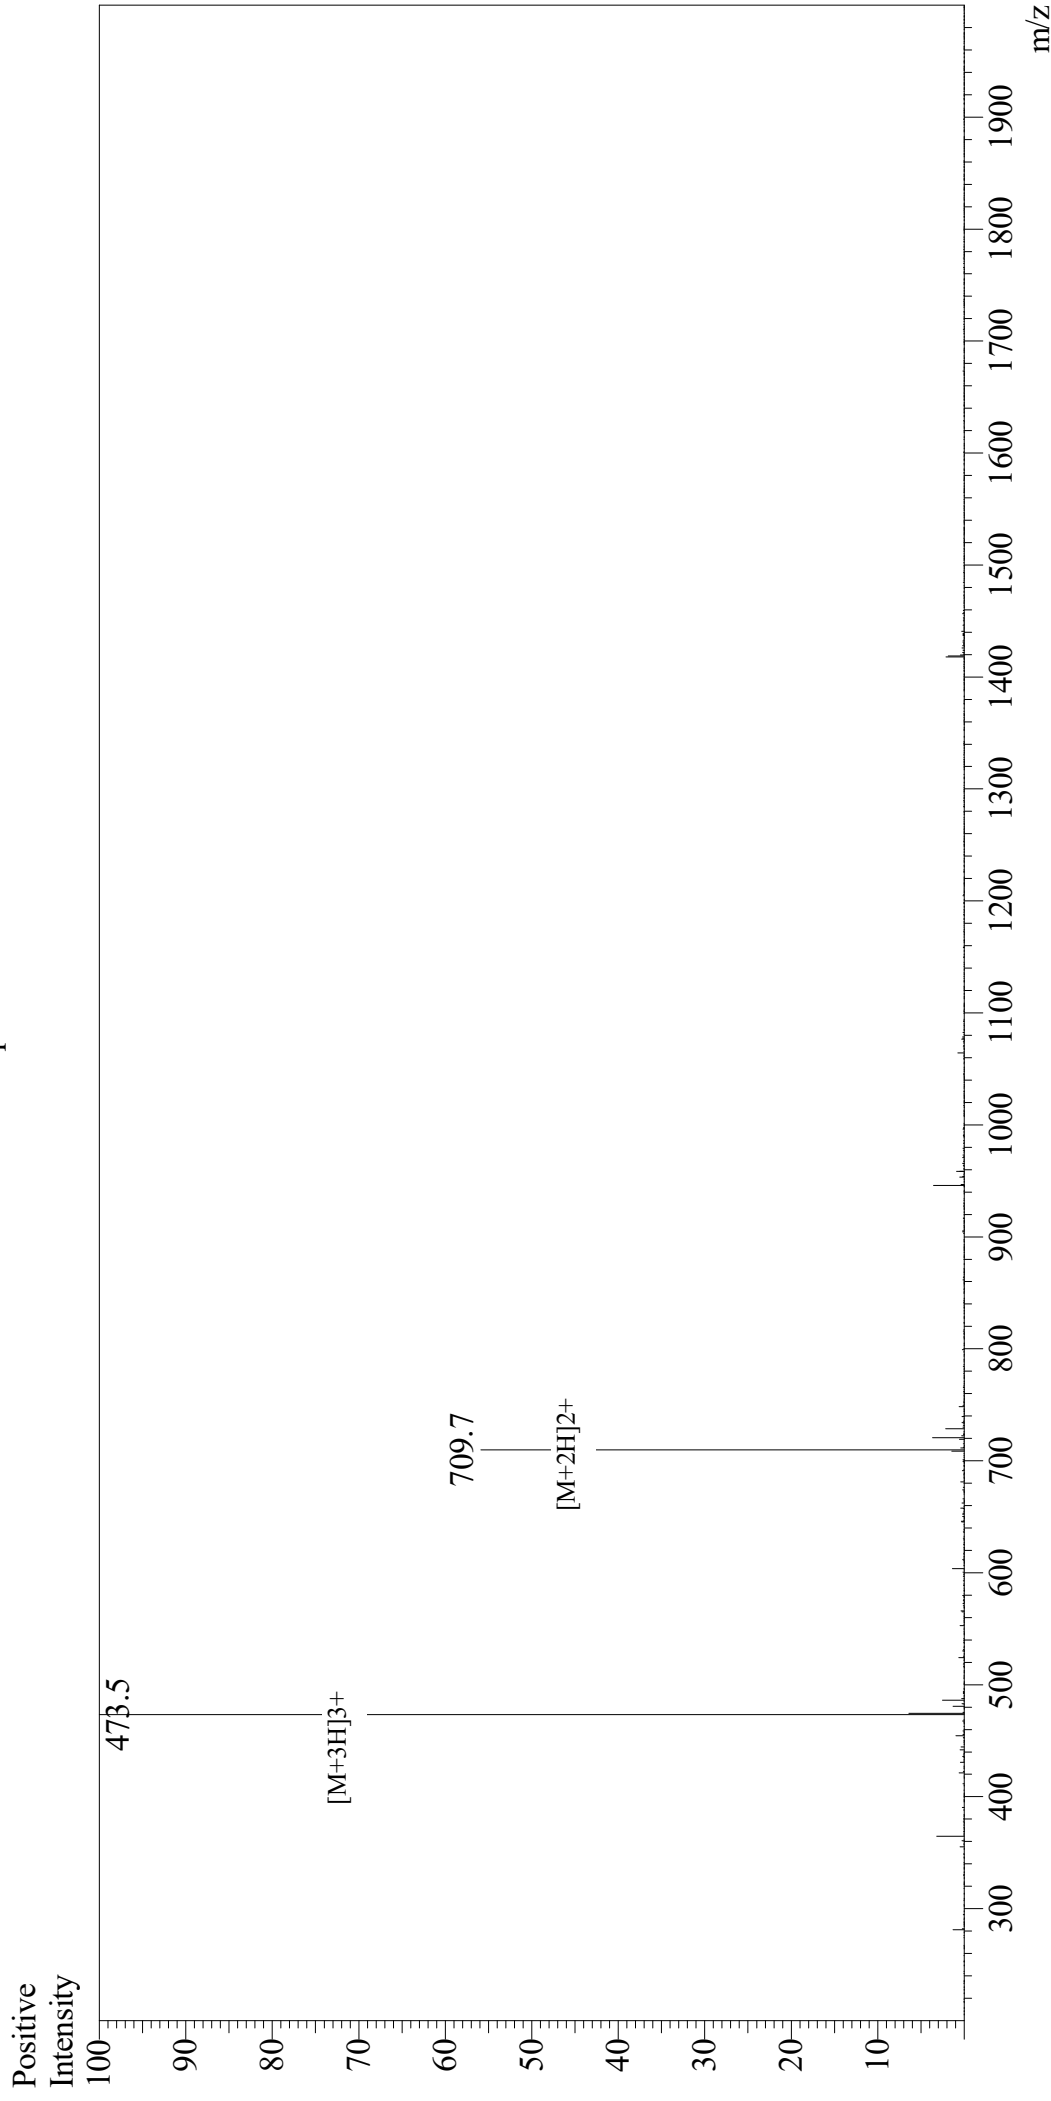

## Sample Information

User : Gary  
Month-Day Processed : 10/04/19  
Time Processed : 10:54:02 AM  
Injection Volume : 0.4  
Sample Name : MARK Substrate  
Cat No. : RP20244  
Lot No. : E7051919J  
Theoretical MW : 1417.61  
Observed MW : 1417.5

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH