

Sample Name :  $\beta$ -Amyloid (1-42), rat  
 Cat No. : RP10013  
 Lot No. : PE4341809  
 Time Processed : 15:57:27  
 Month-Day-Year Processed : 10/09/2018

Pump A : 0.5% Ammonia solution in 100% water (v/v)  
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
37.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment: GR09010180

Chromatogram

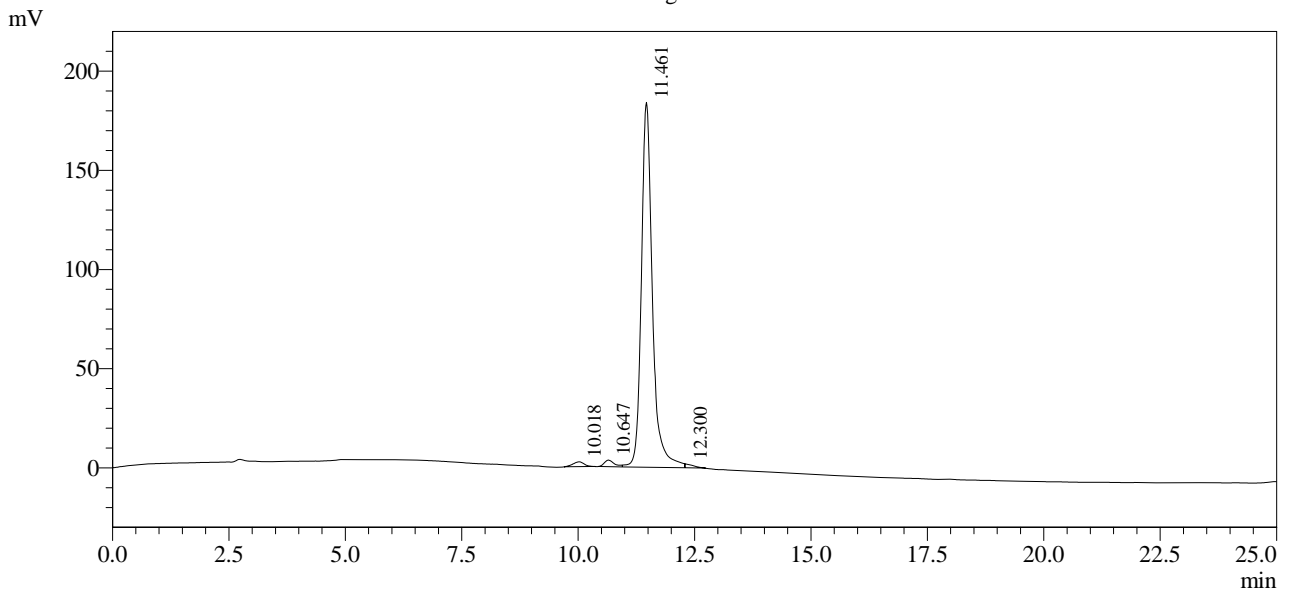

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.018	40913	2434	1.302
2	10.647	49744	3317	1.583
3	11.461	3028711	183965	96.357
4	12.300	23851	1986	0.759
Total		3143218	191702	100.000