

Sample Name : Influenza HA (518-526)
 Cat.No : RP20284
 Lot.No : E4296520L
 Time Processed: 22:33:22
 Year-Month-Day: 2020/12/26

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

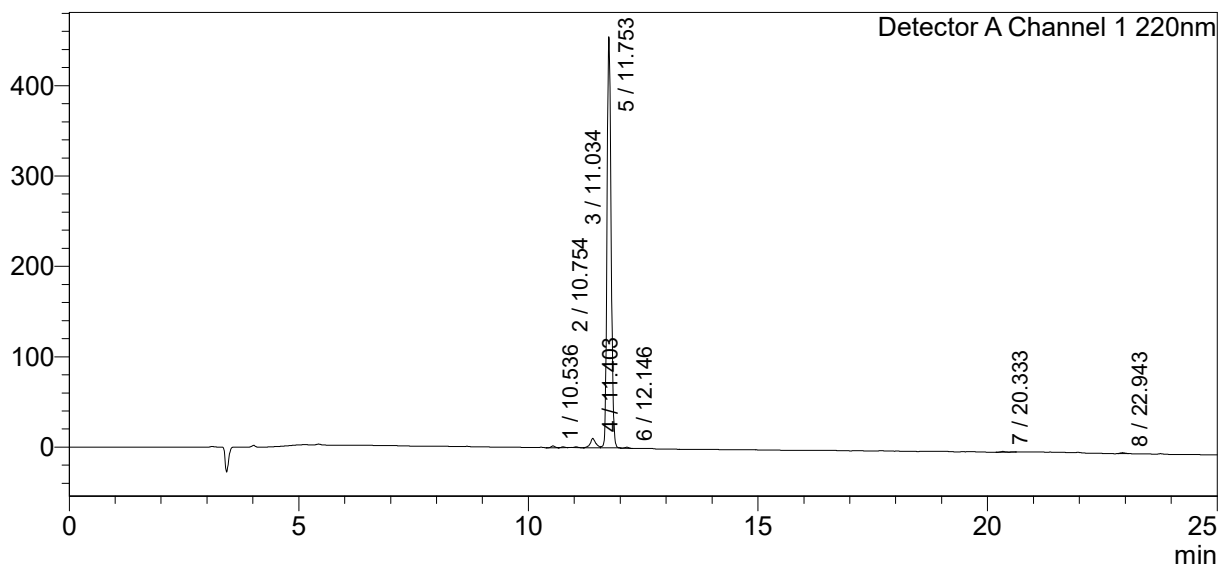

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.536	10185	1952	0.345
2	10.754	4275	870	0.145
3	11.034	4575	896	0.155
4	11.403	86895	10414	2.945
5	11.753	2828001	454860	95.846
6	12.146	5990	1071	0.203
7	20.333	3916	795	0.133
8	22.943	6724	920	0.228
Total		2950562	471777	100.000