

Sample Name :N-Boc-Phe-Leu-Phe-Leu-Phe  
 Cat. No. : RP12950  
 Lot. No. : PE8631902  
 Time Processed : 11:04:01  
 Month-Day-Year Processed : 03/07/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
45.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

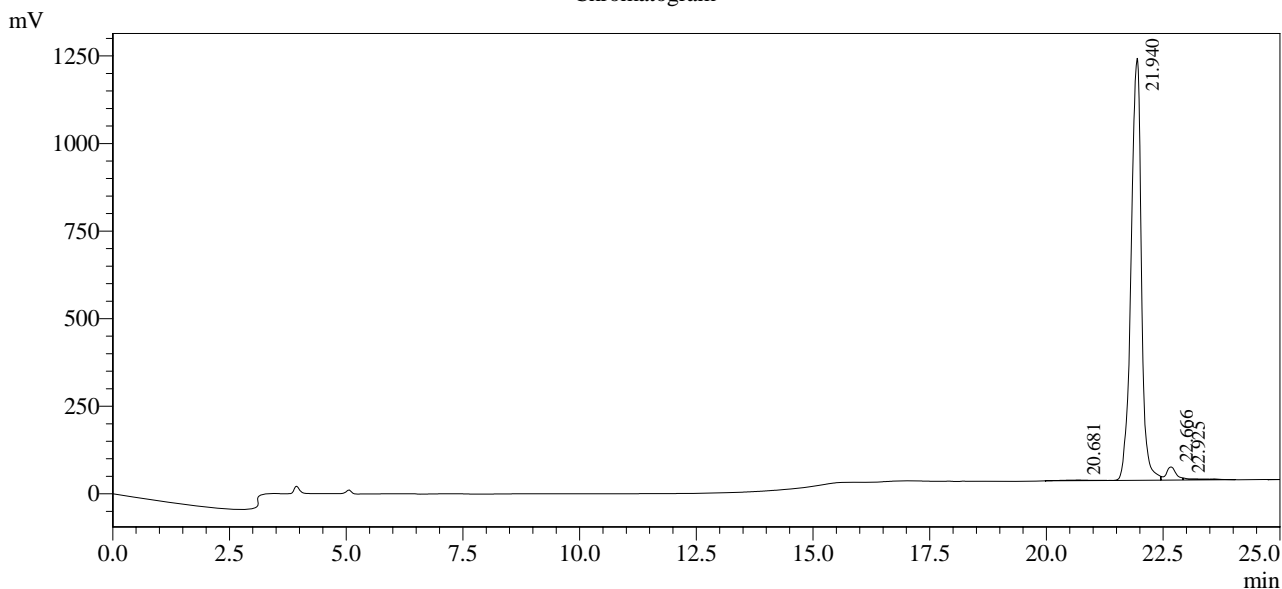

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	20.681	73013	1646	0.379
2	21.940	18381257	1204951	95.502
3	22.666	551888	37405	2.867
4	22.925	139259	6003	0.724
5	25.208	101561	11978	0.528
Total		19246978	1261983	100.000