

Sample Name :Hemorphin-7  
 Cat No. :RP17312  
 Lot No. : E4904919I  
 Time Processed : 19:05:24  
 Month-Day-Year Processed : 09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

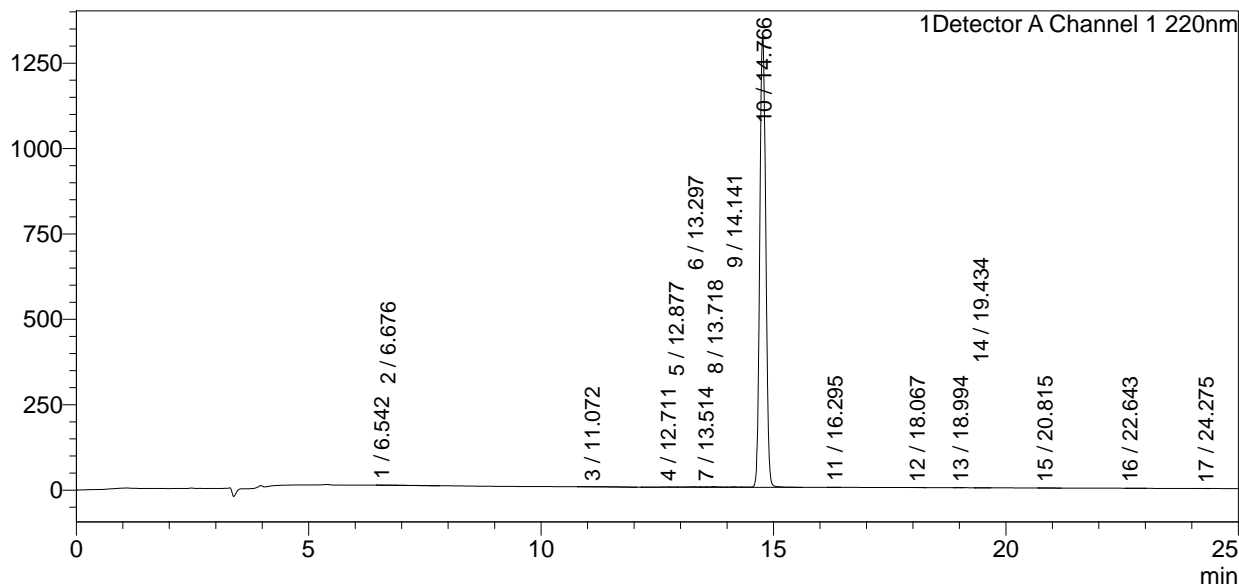

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.542	1054	231	0.009
2	6.676	21286	496	0.178
3	11.072	36482	727	0.304
4	12.711	11381	632	0.095
5	12.877	7413	784	0.062
6	13.297	31444	1535	0.262
7	13.514	7929	1070	0.066
8	13.718	33252	2304	0.277
9	14.141	18966	1692	0.158
10	14.766	11812450	1319576	98.505
11	16.295	1206	133	0.010
12	18.067	1085	128	0.009
13	18.994	1068	217	0.009
14	19.434	1089	110	0.009
15	20.815	2232	164	0.019

Peak#	Ret. Time	Area	Height	Area%
16	22.643	1273	85	0.011
17	24.275	2176	252	0.018
Total		11991786	1330136	100.000