

Sample Name : Oxytocin
 Cat. No. : RP10407
 Lot. No. : PE4291707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

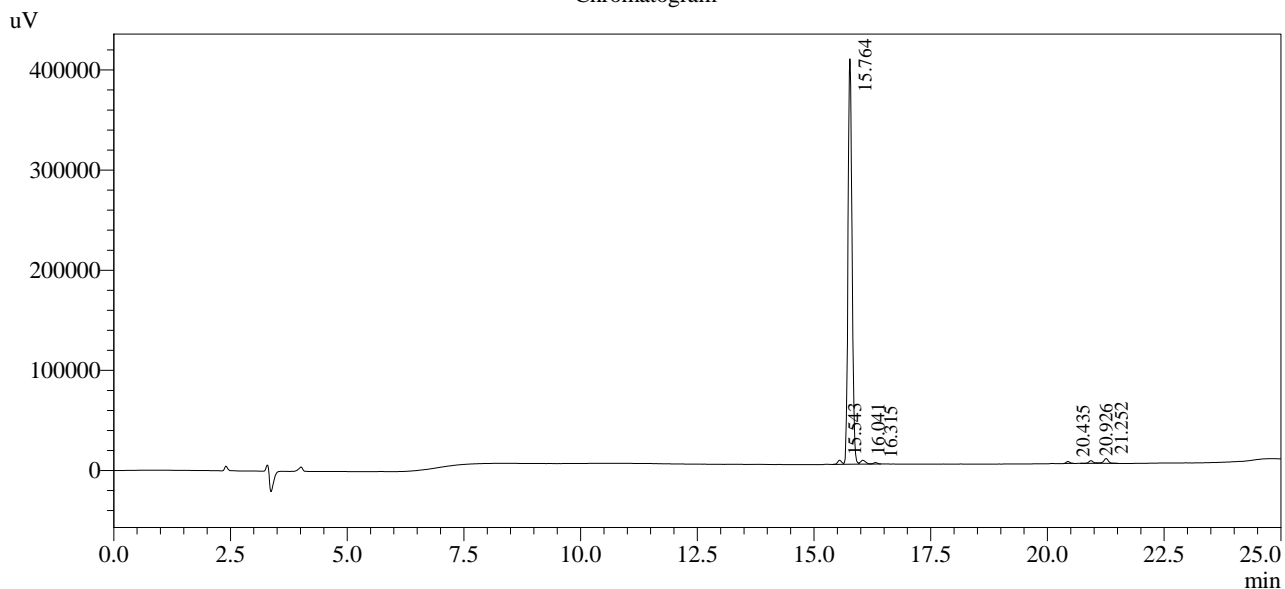

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.543	24353	4115	0.961
2	15.764	2408669	404842	95.014
3	16.041	29447	3815	1.162
4	16.315	8528	1460	0.336
5	20.435	10472	1964	0.413
6	20.926	18210	2705	0.718
7	21.252	35386	4824	1.396
Total		2535065	423724	100.000