

Sample Name :OVA Peptide (257-264)  
 Cat No.: RP10611  
 Lot No.:E6028520K  
 Time Processed :9:05:01  
 Month-Day-Year Processed :11/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

### <Chromatogram>

mV

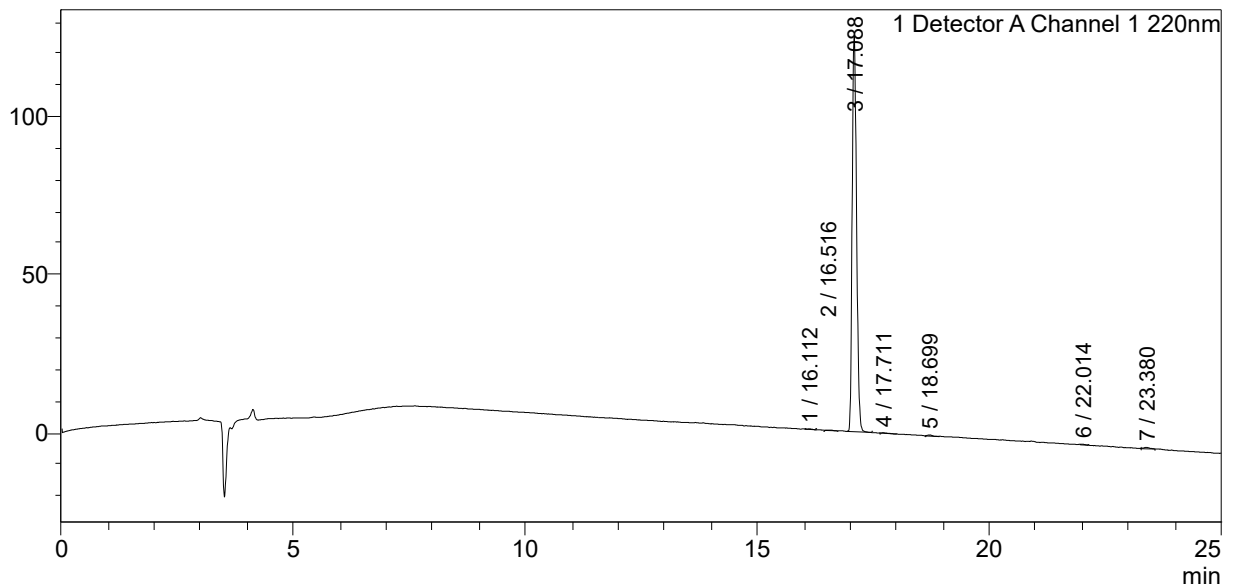

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.112	1175	185	0.141
2	16.516	1006	89	0.121
3	17.088	820952	125253	98.584
4	17.711	1968	177	0.236
5	18.699	2418	301	0.290
6	22.014	1183	246	0.142
7	23.380	4045	435	0.486
Total		832747	126685	100.000