

Sample Name :Bacterial Sortase Substrate III, Abz/DNP  
 Cat. No. : RP20431  
 Lot. No. : PE1851905  
 Time Processed : 9:04:19  
 Month-Day-Year Processed : 05/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

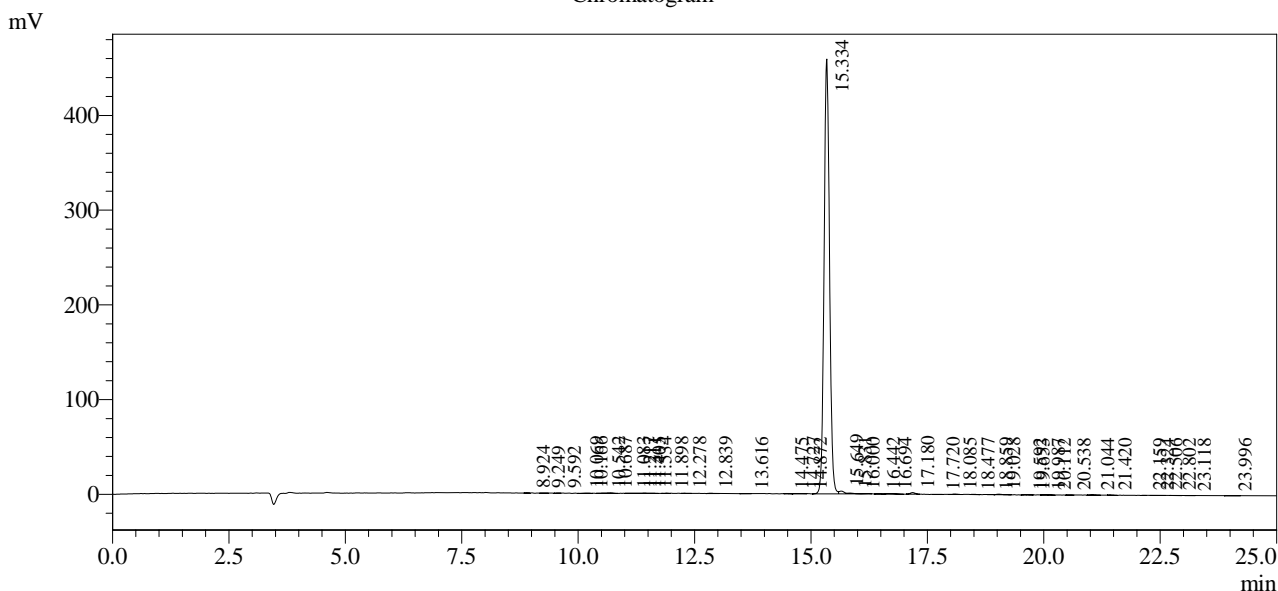

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.924	1329	232	0.034
2	9.249	1632	199	0.042
3	9.592	1015	170	0.026
4	10.069	1176	216	0.030
5	10.166	1889	281	0.049
6	10.542	2831	369	0.073
7	10.687	6135	637	0.158
8	11.083	1735	303	0.045
9	11.217	1667	230	0.043
10	11.311	1139	273	0.029
11	11.405	2665	351	0.069
12	11.534	2133	267	0.055
13	11.898	1454	315	0.038
14	12.278	1323	175	0.034
15	12.839	2838	371	0.073
16	13.616	1278	191	0.033
17	14.475	2148	353	0.055
18	14.727	4442	559	0.115
19	14.872	1393	301	0.036
20	15.334	3743858	458985	96.656
21	15.649	23742	2985	0.613
22	15.831	6642	846	0.171
23	16.000	1655	187	0.043

Peak#	Ret. Time	Area	Height	Area %
24	16.442	1203	174	0.031
25	16.694	6577	547	0.170
26	17.180	12437	1659	0.321
27	17.720	1713	205	0.044
28	18.085	4462	579	0.115
29	18.477	1515	235	0.039
30	18.859	1009	151	0.026
31	19.028	4625	555	0.119
32	19.592	1295	286	0.033
33	19.653	1354	288	0.035
34	19.987	1532	272	0.040
35	20.112	1417	211	0.037
36	20.538	1231	167	0.032
37	21.044	2293	295	0.059
38	21.420	1306	233	0.034
39	22.159	1093	193	0.028
40	22.324	2687	283	0.069
41	22.506	1109	257	0.029
42	22.802	2025	247	0.052
43	23.118	2370	280	0.061
44	23.996	4018	344	0.104
Total		3873388	476258	100.000