

Sample Name :Flagelin22
 Cat No. :RP19986
 Lot No. :E6387319G
 Time Processed :10:11:59
 Month-Day-Year Processed :07/30/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

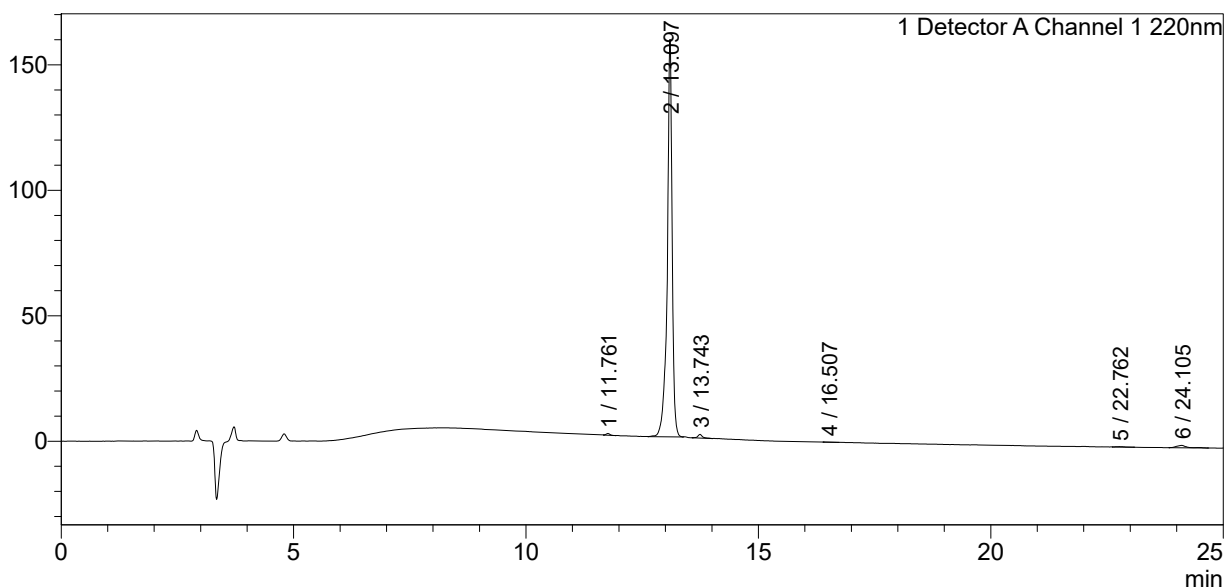

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.761	3674	702	0.312
2	13.097	1147826	158350	97.362
3	13.743	9989	1449	0.847
4	16.507	1219	142	0.103
5	22.762	2476	185	0.210
6	24.105	13743	965	1.166
Total		1178927	161792	100.000