


Mass Spectrum

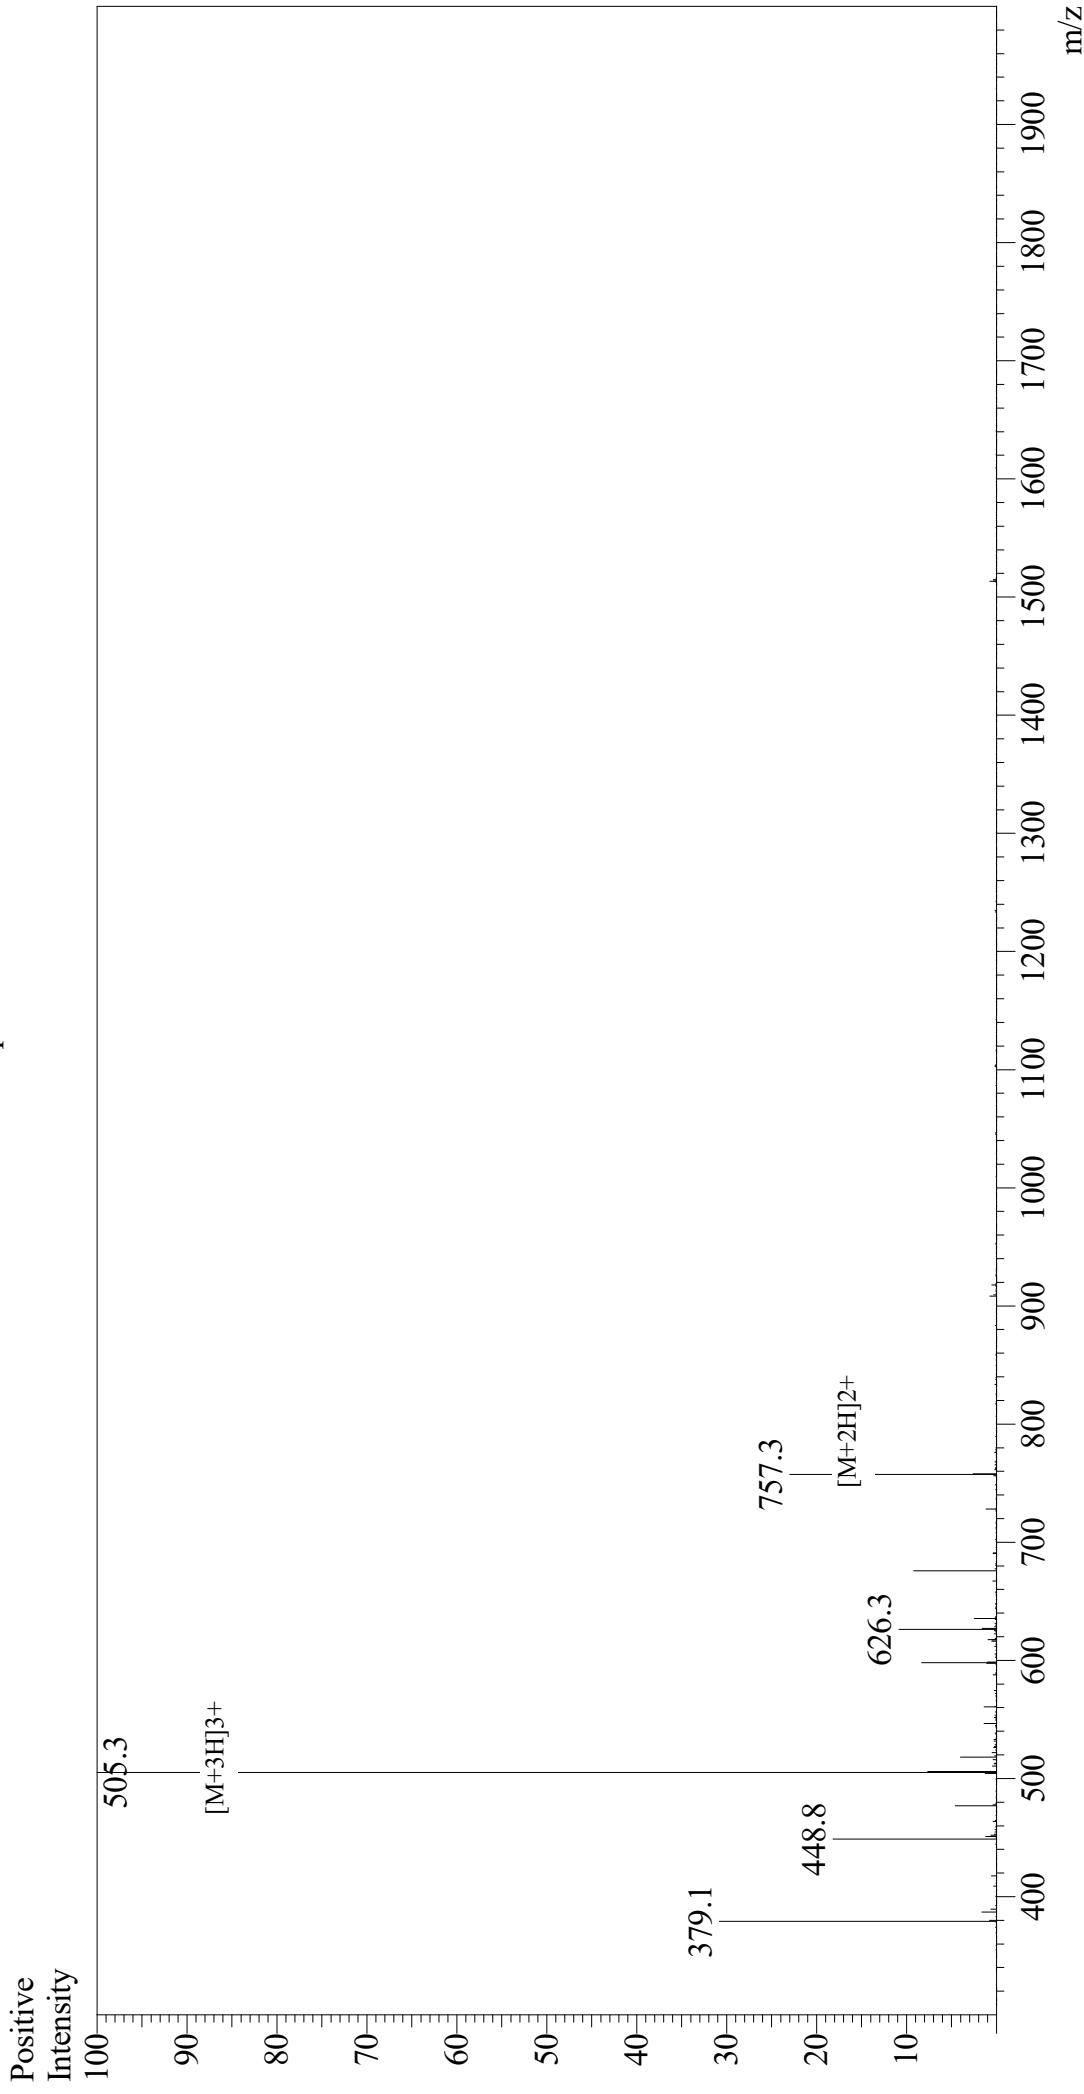

Sample Information

Acquired by : Gary
Month-Day Processed : 08/01/19
Time Processed : 10:32:51 PM
Injection Volume : 0.3
Sample Name : γ -1-Melanocyte Stimulating Hormone (MSH), amide
Cat. No. : RP10650
Lot. No. : E5643819H
Theoretical MW : 1512.90
Observed MW : 1512.9

Interface : ESI

Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH

: GK11010007