

Sample Name : c-Myc Peptide
 Cat. No. : RP11731
 Lot. No. : E5710919F
 Time Processed : 10:23:59
 Month-Day-Year Processed : 06/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

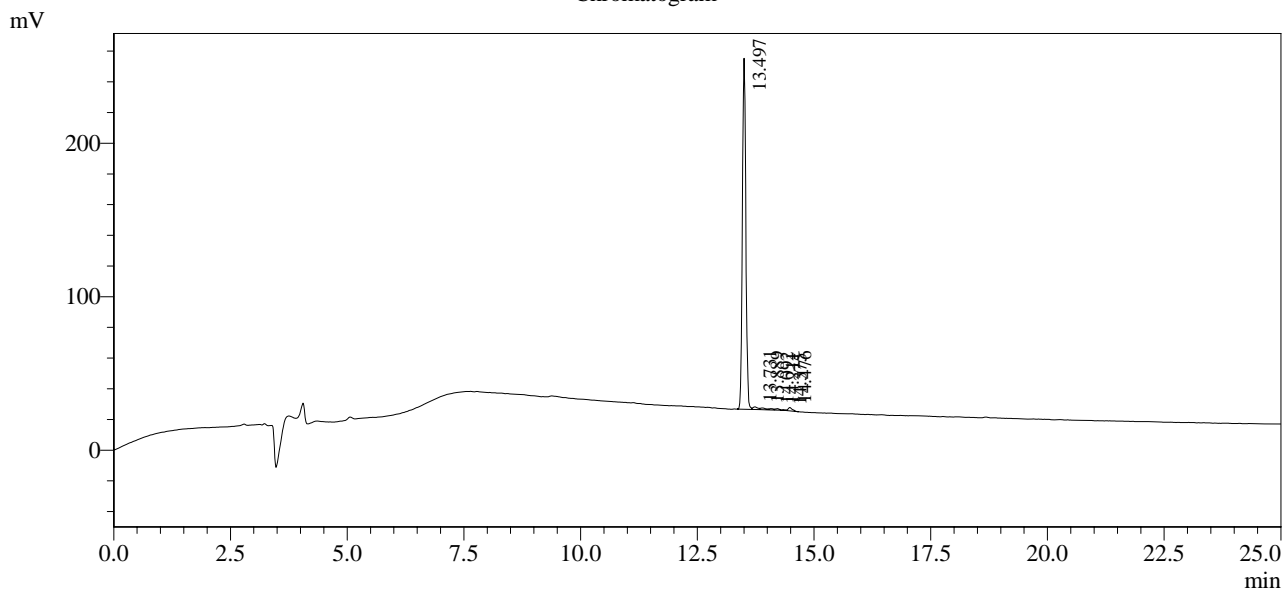

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.497	1177098	228768	96.036
2	13.731	12788	1788	1.043
3	13.889	9884	1167	0.806
4	14.092	5408	812	0.441
5	14.211	5532	962	0.451
6	14.375	1230	349	0.100
7	14.476	13747	2175	1.122
Total		1225688	236022	100.000