

Sample Name :Kallikrein Inhibitor  
 Cat No.: RP10161  
 Lot No.: E6975519J  
 Time Processed :7:18:22  
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

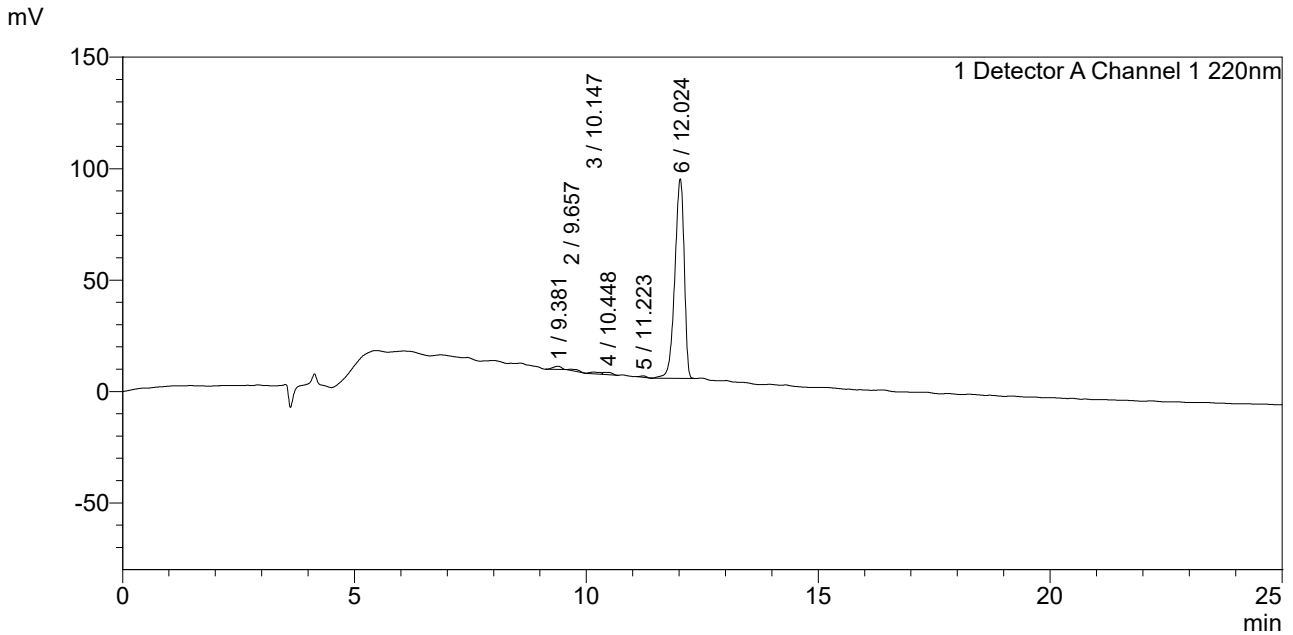

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.381	18181	1445	1.380
2	9.657	11377	538	0.863
3	10.147	12723	729	0.966
4	10.448	13972	1065	1.060
5	11.223	6083	695	0.462
6	12.024	1255248	89627	95.269
Total		1317583	94097	100.000