


Mass Spectrum

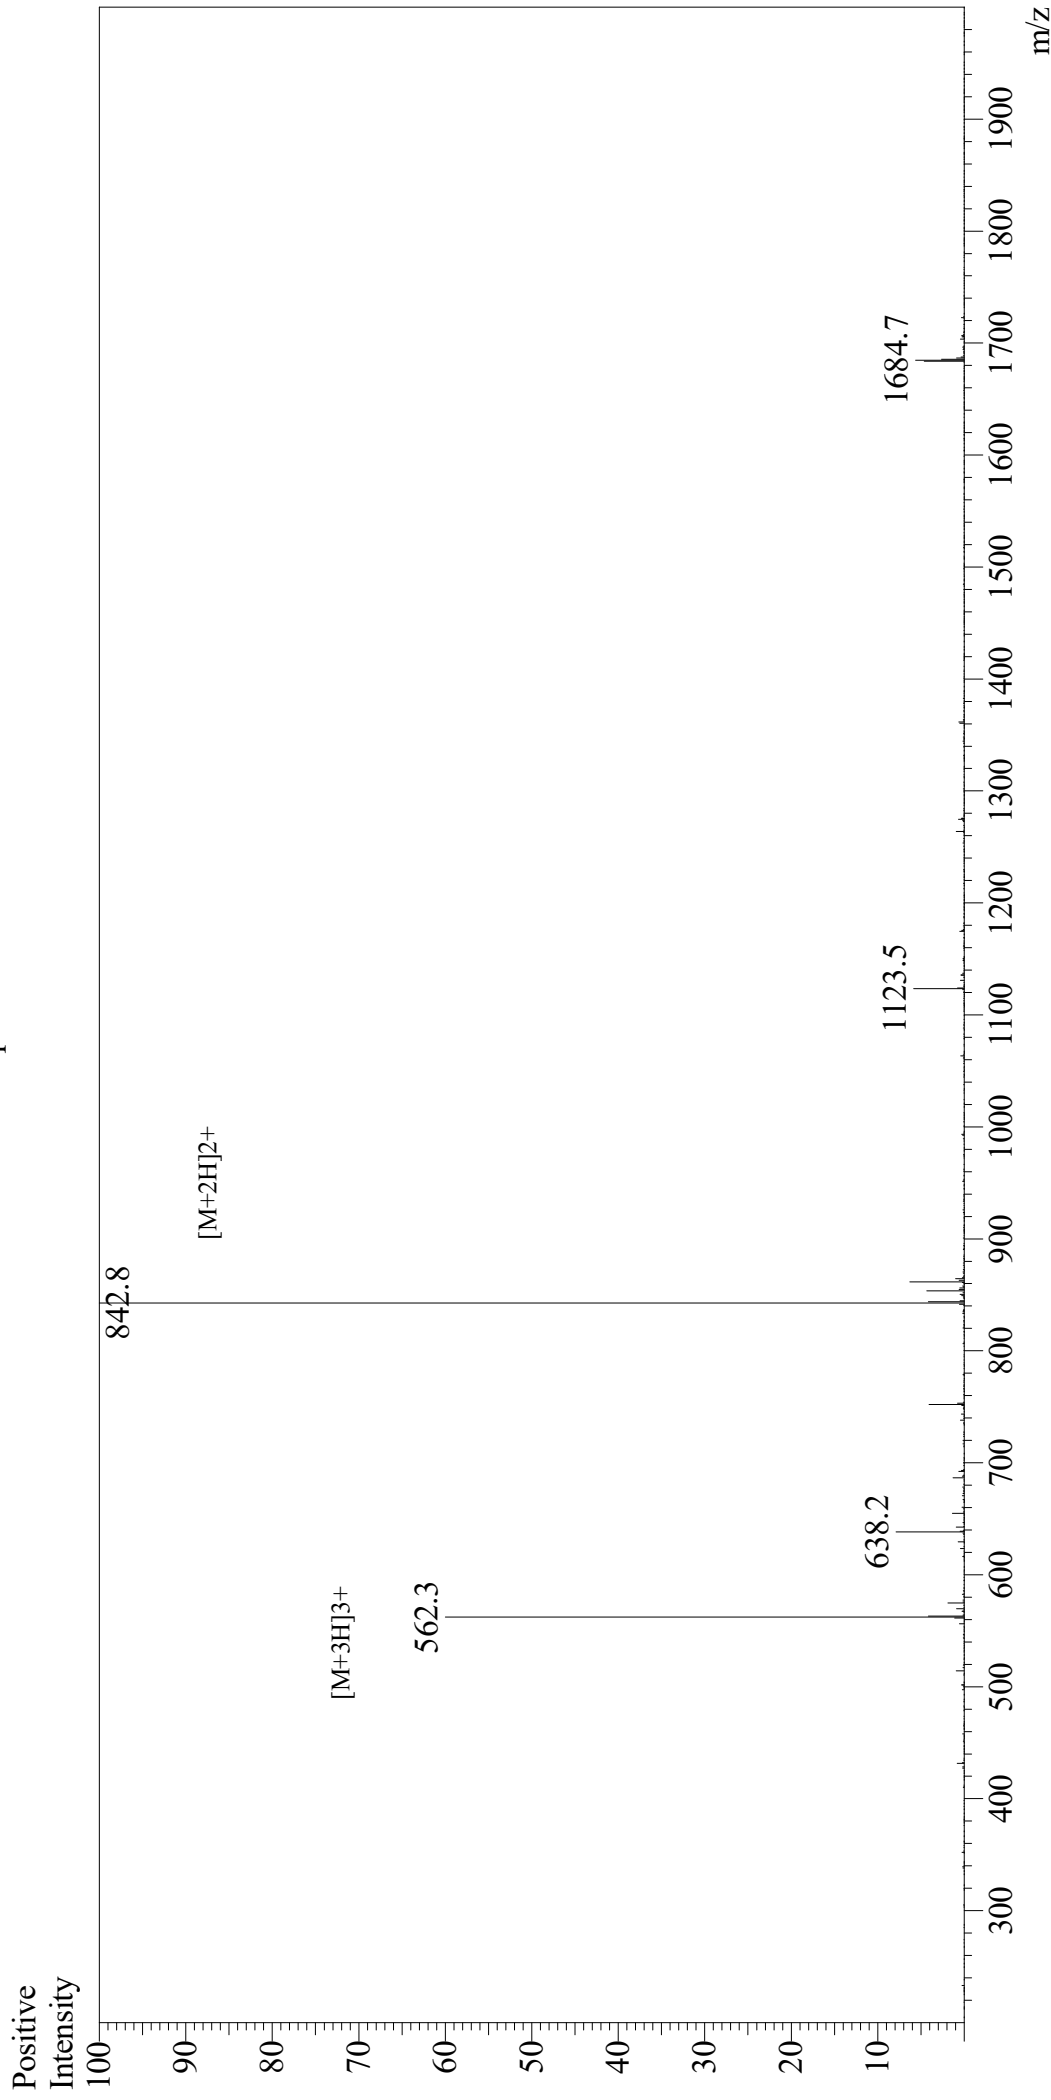

Sample Information

User : Gary
Month-Day Processed : 07/14/20
Time Processed : 09:50:03 PM
Injection Volume : 0.3
Sample Name : α -Factor Mating Pheromone, yeast
Cat No. : RP01002
Lot No. : E9625820G
Theoretical MW : 1683.98
Observed MW : 1683.6

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200