

Sample Name :Angiotensin I, human
 Cat. No. : RP11251
 Lot. No. : E2477820J
 Time Processed :1:45:32 AM

Month-Day-Year Processed :10/16/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

<Chromatogram>

mV

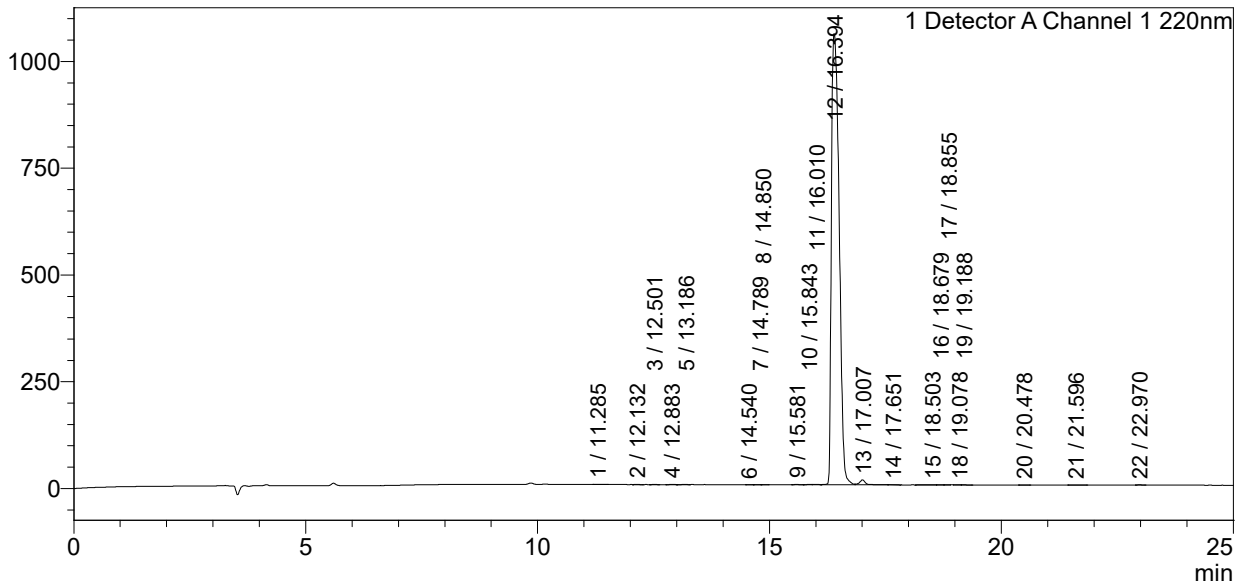

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.285	2232	203	0.018
2	12.132	1154	137	0.009
3	12.501	1335	180	0.011
4	12.883	1900	256	0.015
5	13.186	1876	158	0.015
6	14.540	1090	120	0.009
7	14.789	1579	220	0.013
8	14.850	1182	223	0.010
9	15.581	6757	1078	0.055
10	15.843	6081	909	0.049
11	16.010	9854	1255	0.080
12	16.394	12155888	1056730	98.664
13	17.007	102272	11742	0.830
14	17.651	1651	259	0.013
15	18.503	9960	690	0.081
16	18.679	2673	337	0.022

Peak#	Ret. Time	Area	Height	Area%
17	18.855	1645	238	0.013
18	19.078	2127	279	0.017
19	19.188	1654	251	0.013
20	20.478	2494	248	0.020
21	21.596	2835	224	0.023
22	22.970	2199	340	0.018
Total		12320439	1076075	100.000