

Sample Name :β-MSH, human
 Cat. No. :RP10648
 Lot. No. : PE4301902
 Time Processed : 10:13:07
 Month-Day-Year Processed : 02/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

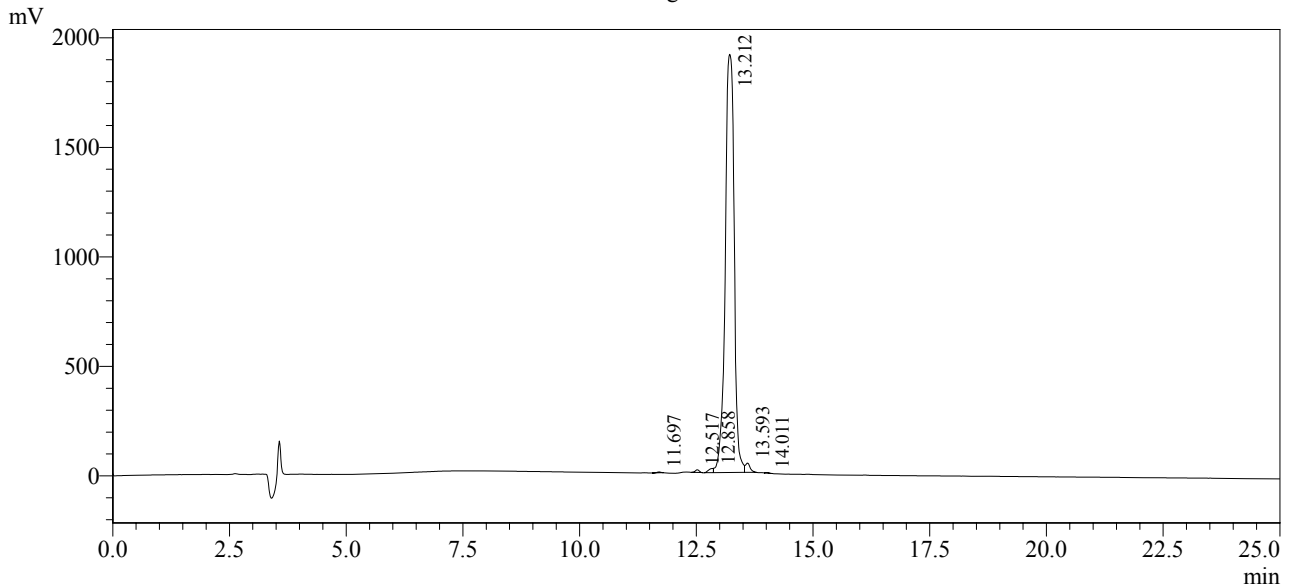

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.697	21336	3952	0.082
2	12.517	71002	12145	0.274
3	12.858	137777	19433	0.531
4	13.212	25395137	1909839	97.915
5	13.593	299615	42763	1.155
6	14.011	11091	2086	0.043
Total		25935957	1990218	100.000