

Sample Name :[Arg8]-Vasopressin (AVP)  
 Cat No. :RP20275  
 Lot No. :E4400221E  
 Time Processed :21:45:30  
 Month-Day-Year Processed :05/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

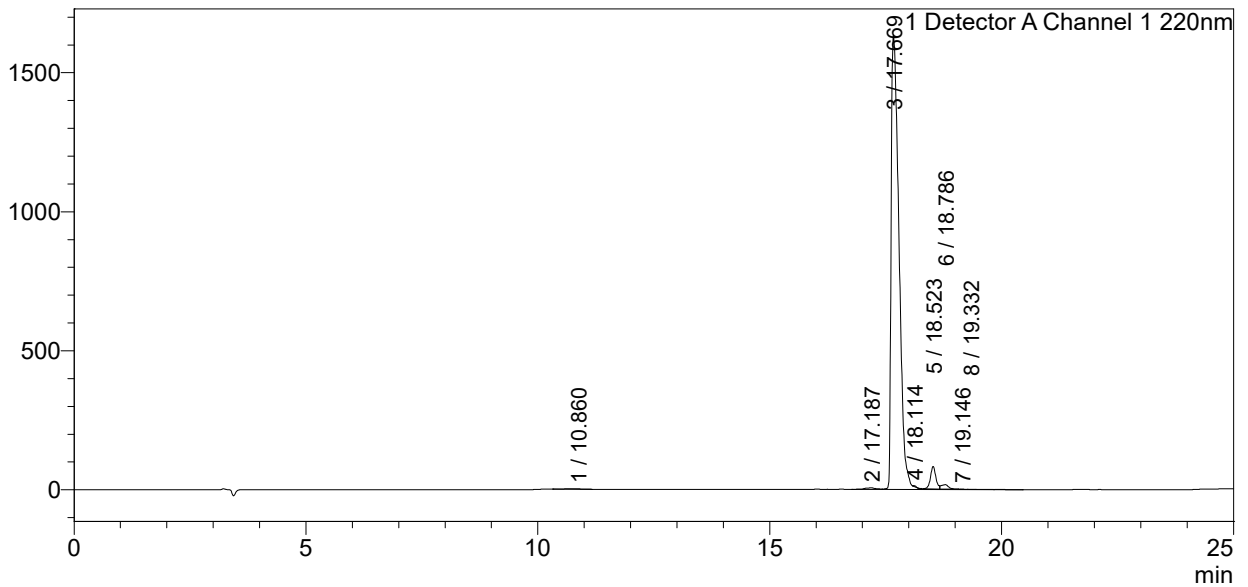

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.860	35332	1676	0.175
2	17.187	91839	5791	0.455
3	17.669	19208513	1635393	95.234
4	18.114	10578	2628	0.052
5	18.523	647842	80469	3.212
6	18.786	171871	15755	0.852
7	19.146	1219	122	0.006
8	19.332	2561	422	0.013
Total		20169754	1742256	100.000