

Sample Name :Influenza Hemagglutinin (307-319)  
 Cat No.: RP20087  
 Lot No.: E5845020C  
 Time Processed :15:52:00  
 Month-Day-Year Processed :03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

### <Chromatogram>

mV

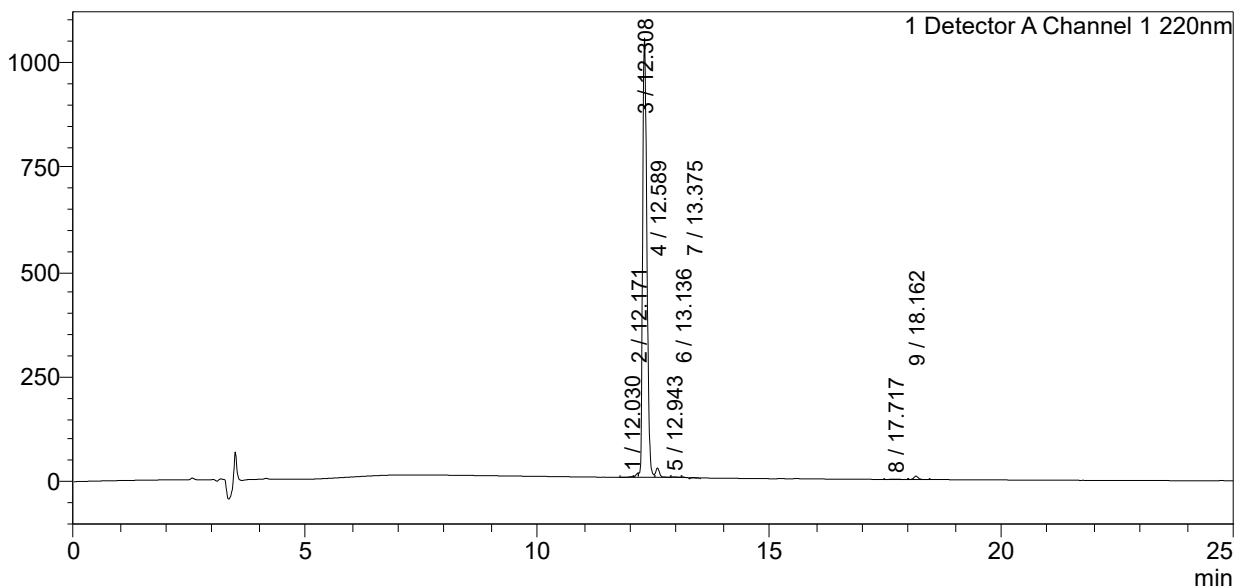

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.030	14051	2194	0.203
2	12.171	39618	10509	0.573
3	12.308	6648232	1049410	96.163
4	12.589	131236	22330	1.898
5	12.943	10971	1492	0.159
6	13.136	5796	1284	0.084
7	13.375	1804	315	0.026
8	17.717	8818	885	0.128
9	18.162	53007	8174	0.767
Total		6913534	1096592	100.000