

Sample Name :Neuropeptide EI, rat  
 Cat No. :RP20309  
 Lot No. :E4921019I  
 Time Processed :14:49:25  
 Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

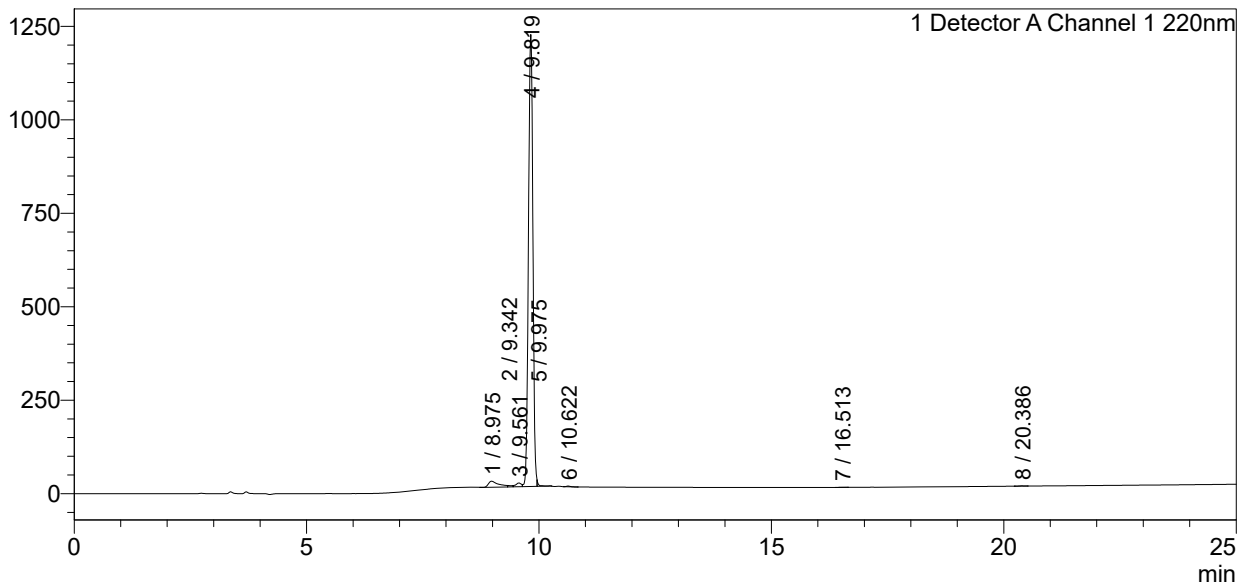

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.975	246466	16026	2.926
2	9.342	23537	3612	0.279
3	9.561	81970	9898	0.973
4	9.819	8024090	1203534	95.261
5	9.975	31806	10677	0.378
6	10.622	9834	1876	0.117
7	16.513	2101	363	0.025
8	20.386	3492	528	0.041
Total		8423296	1246514	100.000