


# Mass Spectrum

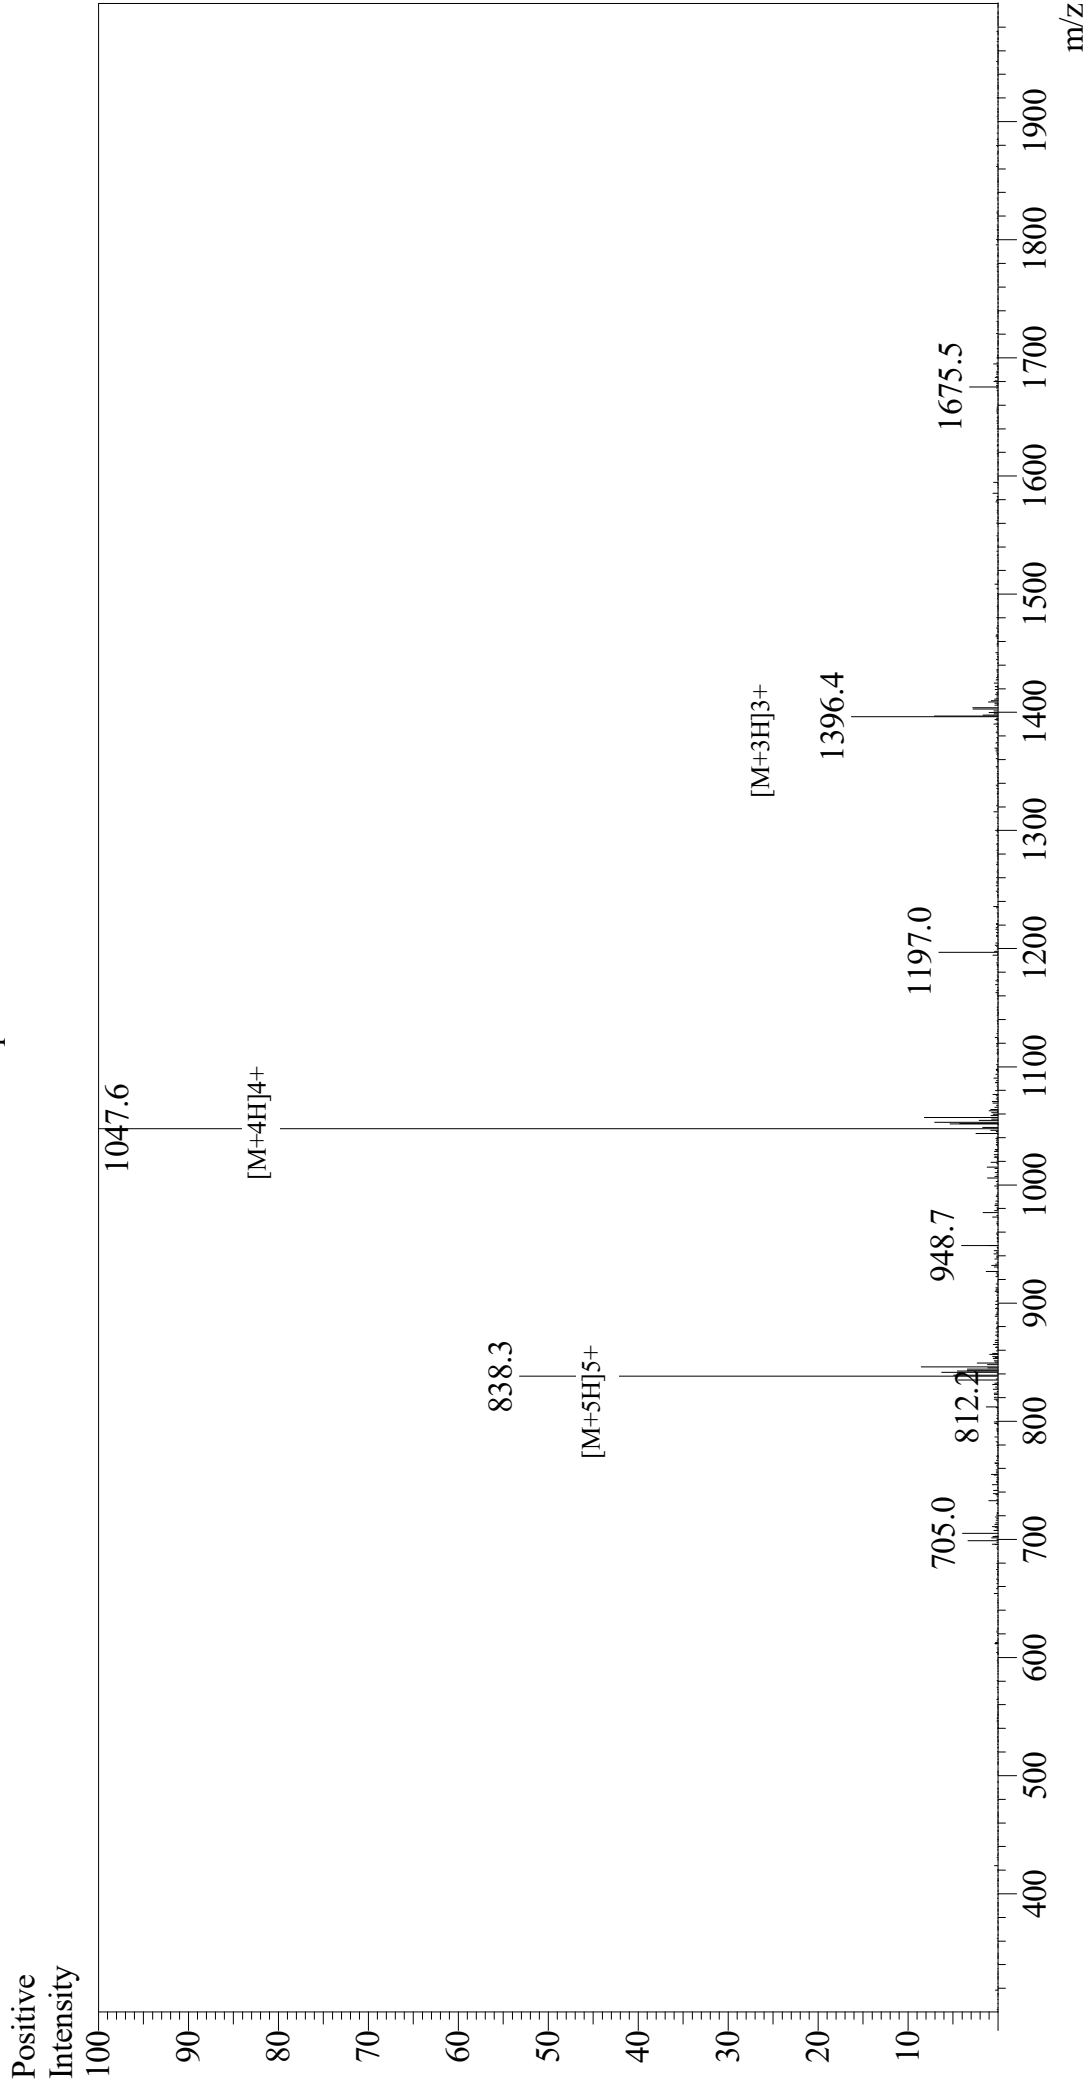

## Sample Information

Acquired by : Gary  
Month-Day Processed : 02/28/20  
Time Processed : 11:54:47 AM  
Injection Volume : 0.5  
Sample Name : Exendin-4  
Cat. No. : RP10874  
Lot. No. : E4781920B  
Theoretical MW : 4186.66  
Observed MW : 4186.4

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50% $\text{H}_2\text{O}$ /50% $\text{MeOH}$