

Sample Name :G3-C12
 Cat No.: RP20329
 Lot No.:E4046719K
 Time Processed :15:21:41
 Month-Day-Year Processed :11/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 15 |
| 25.00 | Pumps | Solvent B Conc. | 75 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 31.00 | Pumps | Solvent B Conc. | 95 |
| 31.01 | Pumps | Solvent B Conc. | 15 |
| 40.00 | Pumps | Solvent B Conc. | 15 |
| 41.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

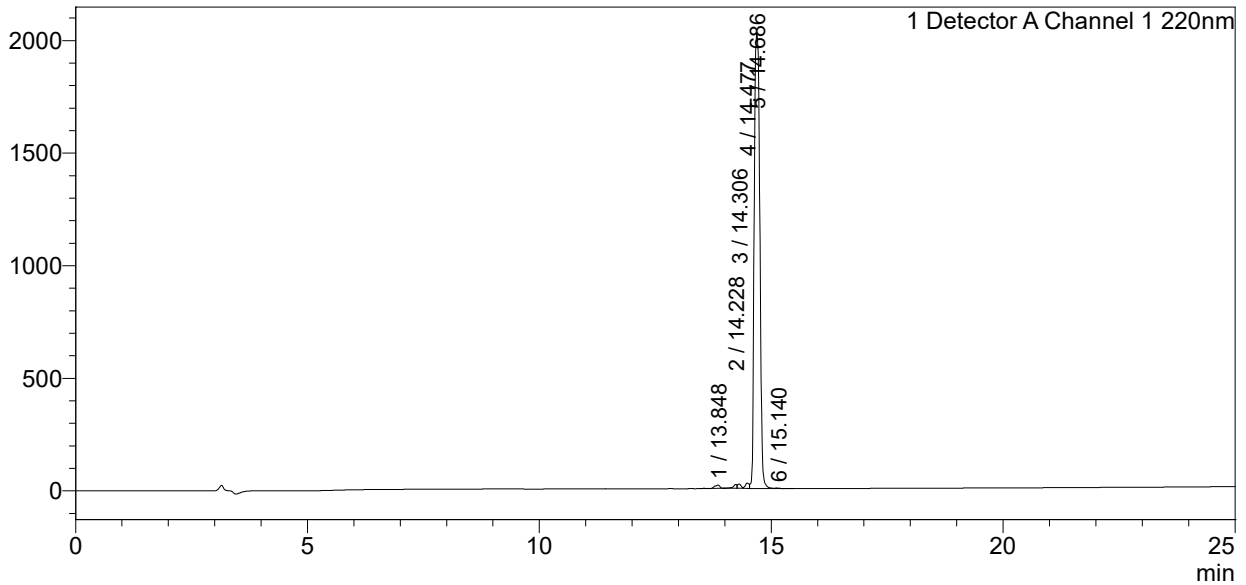

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 1 | 13.848 | 119991 | 14809 | 0.691 |
| 2 | 14.228 | 103778 | 17051 | 0.598 |
| 3 | 14.306 | 96866 | 19243 | 0.558 |
| 4 | 14.477 | 136129 | 23406 | 0.784 |
| 5 | 14.686 | 16898910 | 2023219 | 97.360 |
| 6 | 15.140 | 1452 | 332 | 0.008 |
| Total | | 17357127 | 2098061 | 100.000 |