

Sample Name :Oxytocin  
 Cat No. :RP10407  
 Lot No. :PE5241901  
 Time Processed :9:44:25  
 Month-Day-Year Processed :01/12/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

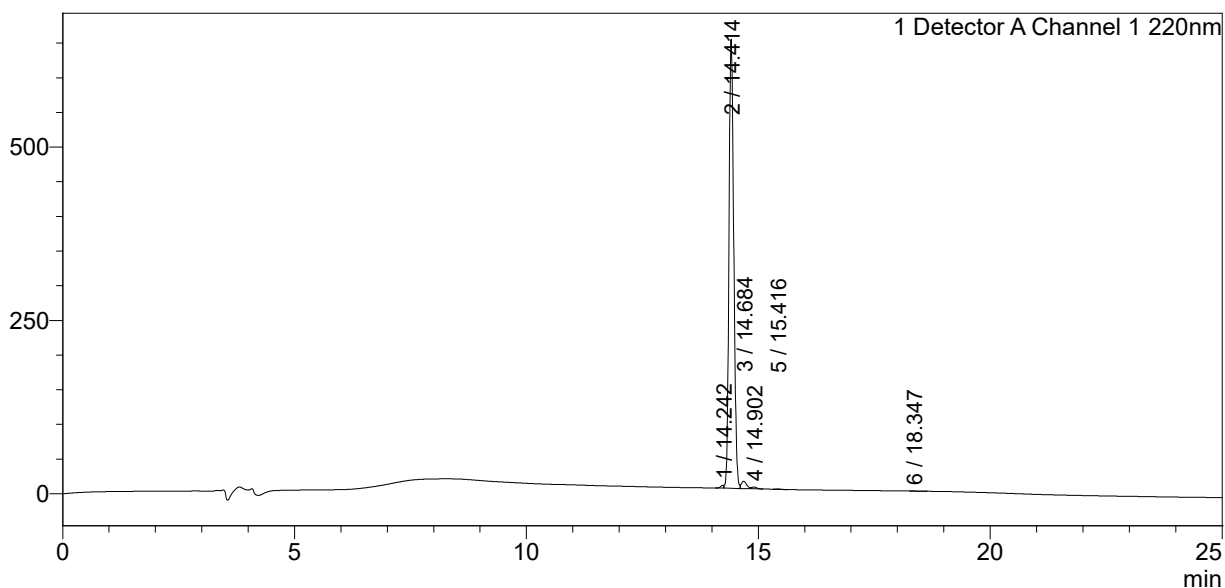

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.242	19407	4057	0.406
2	14.414	4657459	648032	97.338
3	14.684	82617	10460	1.727
4	14.902	19295	2659	0.403
5	15.416	4201	593	0.088
6	18.347	1850	166	0.039
Total		4784827	665968	100.000