

Sample Name : HA Peptide
 Cat No.: RP11735
 Lot No.: E9967420F
 Time Processed : 8:55:10
 Month-Day-Year Processed : 06/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

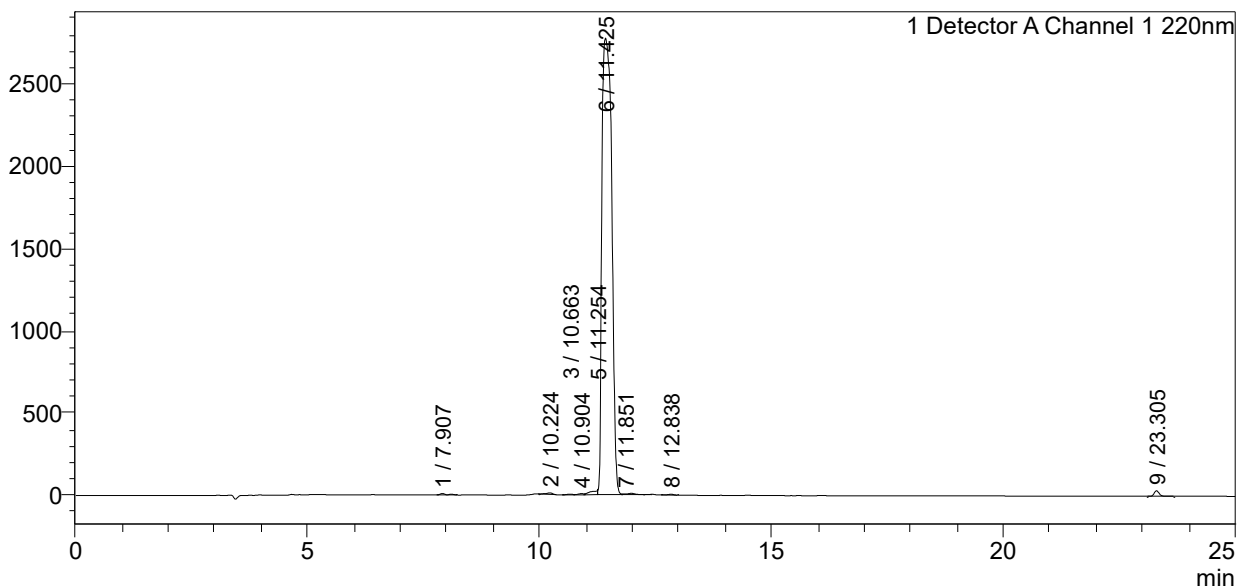

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.907	90587	8991	0.218
2	10.224	76423	8659	0.184
3	10.663	39475	3985	0.095
4	10.904	55676	6666	0.134
5	11.254	291847	24411	0.702
6	11.425	40647971	2774903	97.790
7	11.851	77178	4531	0.186
8	12.838	41664	4531	0.100
9	23.305	245574	33024	0.591
Total		41566393	2869700	100.000