

Sample Name :Substance P
 Cat No. :RP10178
 Lot No. :E9219821J
 Time Processed :23:28:33
 Month-Day-Year Processed :11/08/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

<Chromatogram>

mV

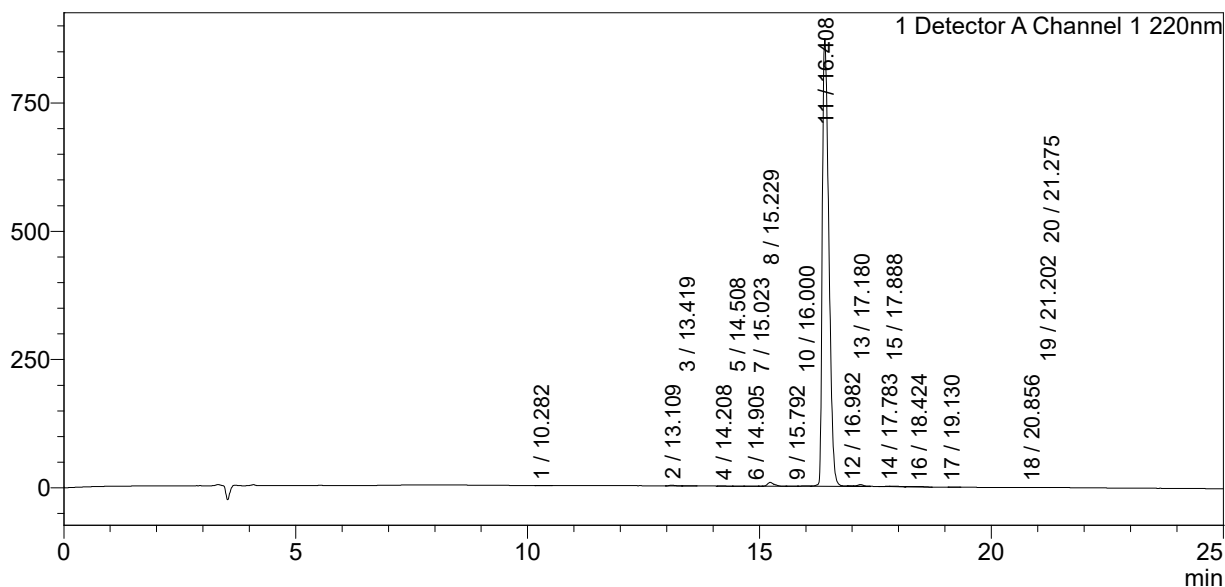

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.282	1268	142	0.015
2	13.109	9918	1361	0.114
3	13.419	1544	214	0.018
4	14.208	1420	149	0.016
5	14.508	1459	182	0.017
6	14.905	2289	227	0.026
7	15.023	1058	226	0.012
8	15.229	75620	7678	0.869
9	15.792	1682	178	0.019
10	16.000	8678	682	0.100
11	16.408	8523367	872471	97.979
12	16.982	2149	359	0.025
13	17.180	26861	3120	0.309
14	17.783	7288	1041	0.084
15	17.888	13166	1158	0.151
16	18.424	12750	799	0.147

Peak#	Ret. Time	Area	Height	Area%
17	19.130	1617	180	0.019
18	20.856	1317	163	0.015
19	21.202	2165	282	0.025
20	21.275	3592	250	0.041
Total		8699209	890861	100.000