

Sample Name :Gly-Arg-Gly-Asp-Asn-Pro
 Cat No. :RP10847
 Lot No. :E5495121H
 Time Processed :22:00:35
 Month-Day-Year Processed :08/17/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

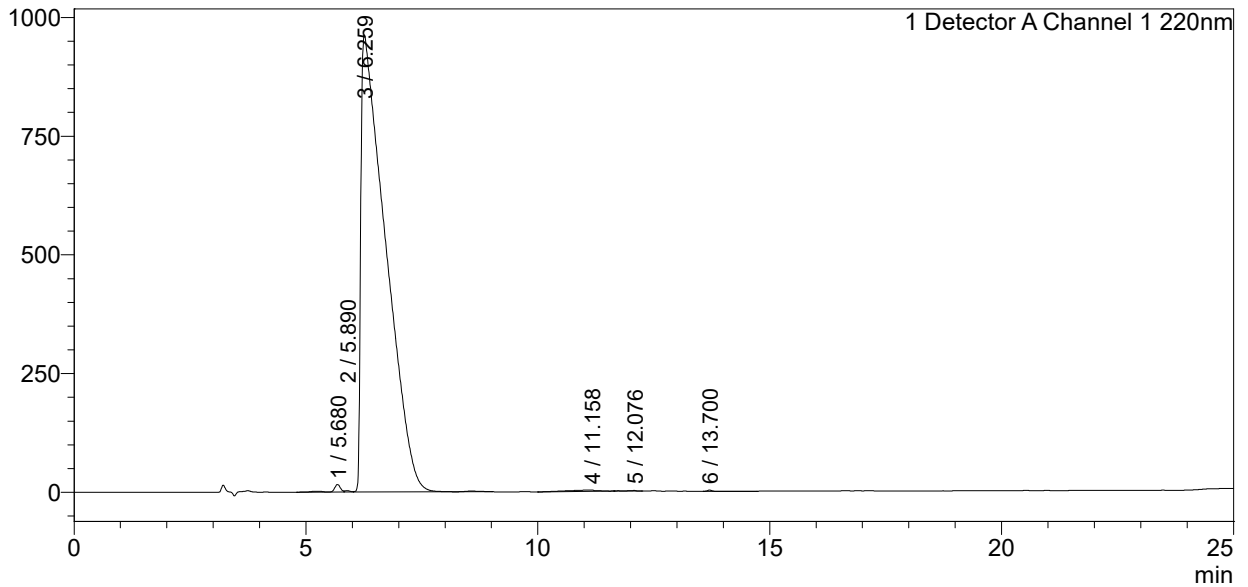

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.680	174565	16049	0.486
2	5.890	23297	3018	0.065
3	6.259	35609702	963244	99.056
4	11.158	116594	2808	0.324
5	12.076	15229	1345	0.042
6	13.700	9640	2557	0.027
Total		35949027	989022	100.000