

Sample Name : Influenza A NP(366 - 374) Strain A/PR/8/35
 Cat No : RP20267
 Lot No : E7687021D
 Time Processed : 9:07:51 PM
 Month-Day-Year Processed : 04/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

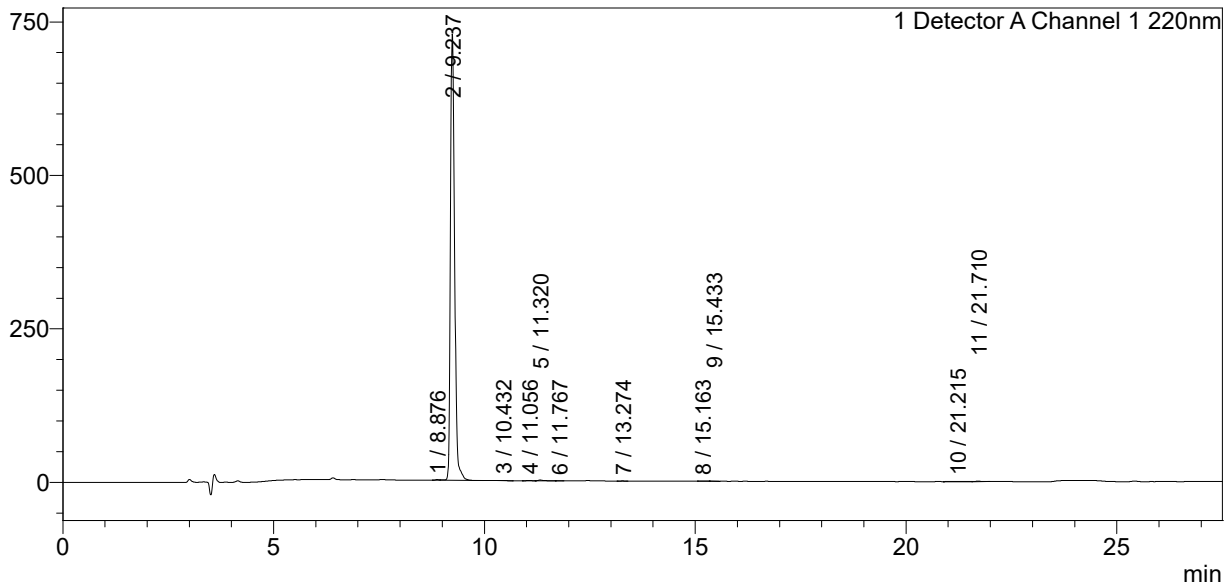

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.876	6444	1022	0.127
2	9.237	5034120	716127	98.908
3	10.432	2833	379	0.056
4	11.056	4310	595	0.085
5	11.320	10979	1261	0.216
6	11.767	1107	195	0.022
7	13.274	2080	345	0.041
8	15.163	2239	279	0.044
9	15.433	1178	187	0.023
10	21.215	17080	543	0.336
11	21.710	7344	649	0.144
Total		5089713	721581	100.000