

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human  
 Cat No.: RP11110  
 Lot No.: E3974720I  
 Time Processed :9:43:52  
 Month-Day-Year Processed :09/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

### <Chromatogram>

mV

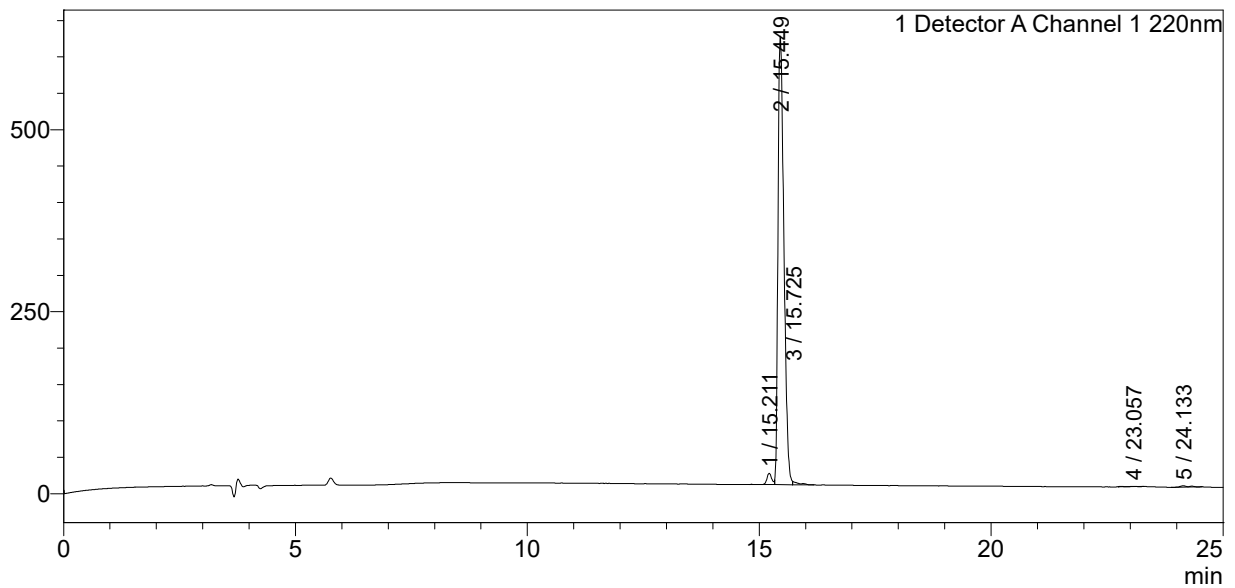

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.211	111874	15542	1.992
2	15.449	5440851	616386	96.894
3	15.725	39728	4403	0.707
4	23.057	1512	432	0.027
5	24.133	21307	1831	0.379
Total		5615272	638593	100.000