

Sample Name : c-Myc Peptide
 Cat. No. : RP11731
 Lot. No. : E4778320H
 Time Processed :17:04:18
 Month-Day-Year Processed :08/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

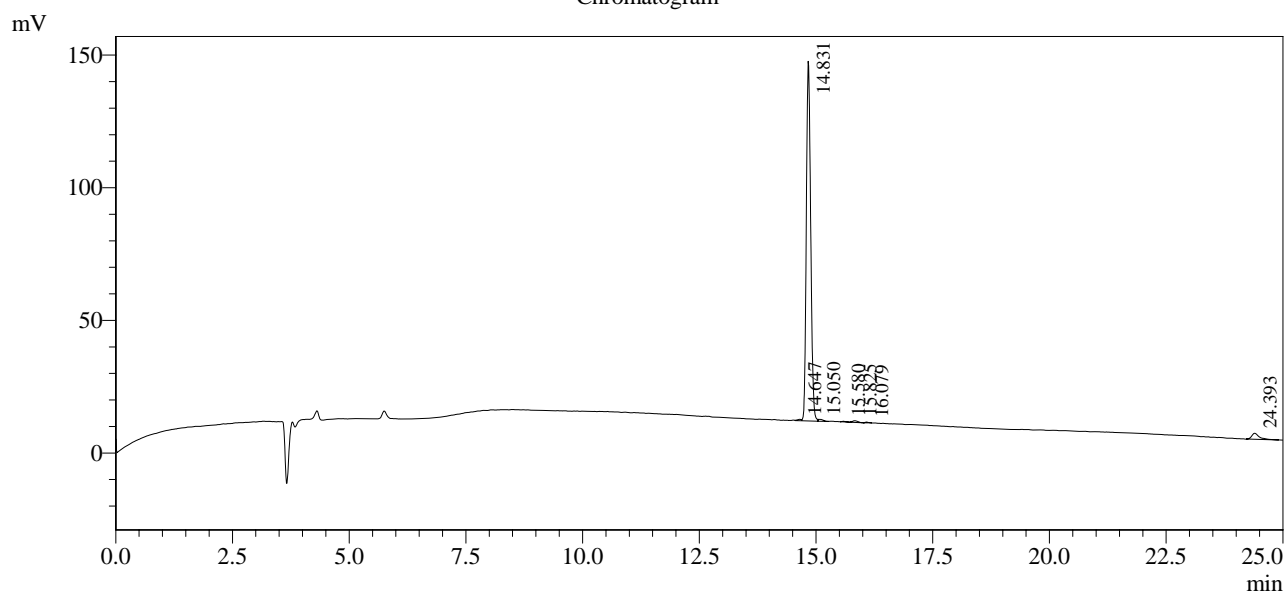

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.647	3201	528	0.349
2	14.831	876832	135602	95.592
3	15.050	5083	718	0.554
4	15.580	1123	209	0.122
5	15.825	4646	606	0.507
6	16.079	1311	280	0.143
7	24.393	25068	2254	2.733
Total		917266	140197	100.000