

Sample Name : γ -2-MSH (41-58), amide
 Cat No.: RP20307
 Lot No.: E5744620B
 Time Processed : 15:45:32
 Month-Day-Year Processed : 02/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
41.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

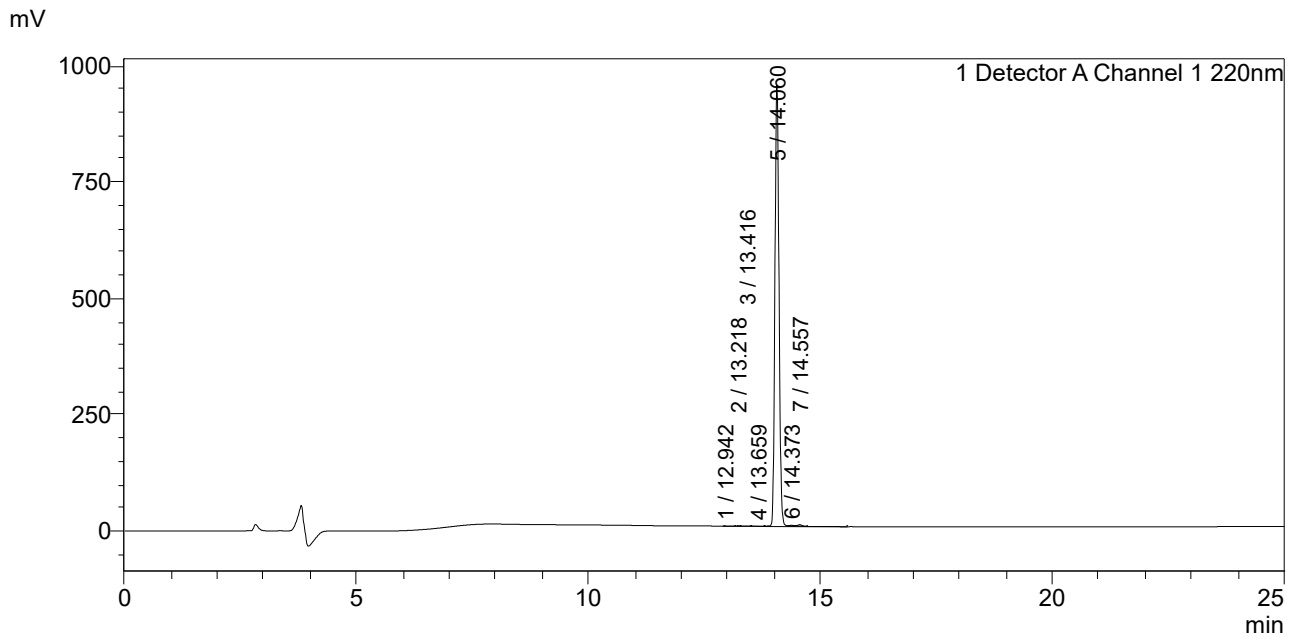

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.942	992	50	0.017
2	13.218	112	25	0.002
3	13.416	2409	313	0.041
4	13.659	5181	593	0.089
5	14.060	5783399	948963	99.329
6	14.373	5741	1178	0.099
7	14.557	24659	3204	0.424
Total		5822493	954326	100.000